

2


R.S. Henderson et al. / Nuclear Instruments and Methods in Physics Research A ■ (■■■■) ■■■-■■■

1 muons [2] pass through a gas degrader and a foil
 2 degrader, which fine tune the muon energy, so that
 3 they pass through the first half of the spectrometer
 4 and stop in a target at the center.

5 TWIST will measure, for the first time, all muon
 6 decay parameters simultaneously, and will do so
 7 by recording two dimensional (momentum and
 8 angle) distributions of the decay positrons.

11 2. Overview

13 Fig. 1 is a conceptual view of the TWIST
 14 spectrometer. The superconducting solenoid has
 15 an inner diameter of 100cm and a length of
 16 223 cm. There are eight drift-chamber (DC)
 17 modules in each half of the spectrometer, for a
 18 total of 44 drift planes. These 16 DC modules
 19 are the main tracking elements of the TWIST
 20 spectrometer. At the upstream and downstream
 21 ends of the stack there are two proportional chamber
 22 (PC) modules, each having four MWPC planes.
 23 The target module, at the center of the spectrometer,
 24 is a somewhat similar MWPC, but with the target
 25 foil acting as the central cathode. The twenty-two
 26 drift chamber layers and six MWPC layers are
 27 positioned both upstream and downstream of the

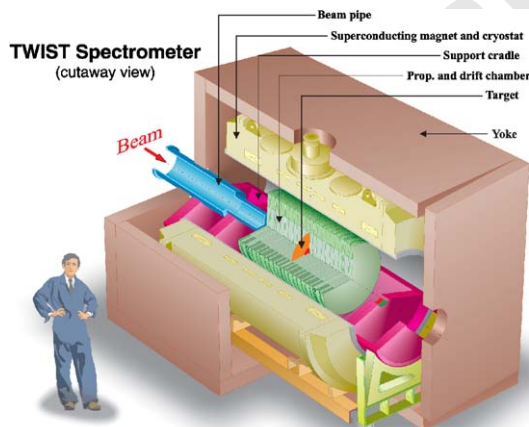


31 Fig. 1. Conceptual drawing of the TWIST spectrometer. It
 32 shows the superconducting solenoid within the steel yoke, with
 33 the drift chambers and proportional chambers symmetrically
 34 placed from the central target.

49 muon stopping target, in a highly symmetrical
 50 pattern.

51 An external steel yoke was required to produce
 52 the highly uniform two Tesla axial field for the DC
 53 tracking volume. This yoke was modeled with
 54 OPERA-3d, then fabricated. It is 20 cm thick at
 55 the top and sides, and 8 cm thick at the ends. The
 56 downstream end of the yoke is hinged for easier
 57 access.

58 Fig. 2 shows two field maps for the typical
 59 operating strength of 2.00 Tesla. The upper plot
 60 shows the field map on the beam axis ($x = y = 0$),
 61 the lower plot shows the field at a radius of
 62 165 mm, at the edge of the tracking volume.
 63 Within this tracking DC volume ($|z| < 500$ mm,
 64 $r < 160$ mm), the measurements determine the
 65 variations of the field as a function of position to
 66 ± 1 gauss. It is uniform over the full volume to
 67 80 G (full width). It has also been mapped at 1.96
 68 and 2.04 T.

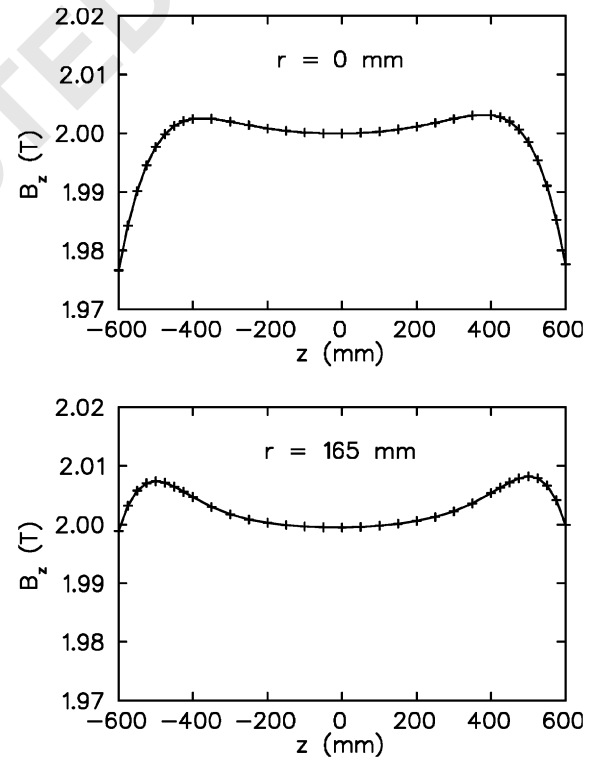

81 Fig. 2. Maps of axial magnetic field, showing B_z vs. z for $x =$
 82 $y = 0$ (upper) and $r = 165$ mm (lower).
 83
 84
 85
 86
 87
 88
 89
 90
 91
 92
 93
 94
 95

Fig. 3 shows a side section view of the TWIST detector stack and the cradle that contains them. The 19 modules are compressed against the upstream end of the cradle by four custom built pneumatic cylinders (see Sections 3 and 8).

To measure the muon decay parameters with the proposed precisions, specific requirements must be met for; chamber resolution, precision of individual chamber construction, and precision of wire-plane positioning (especially in the z direction).

With 44 drift-chamber layers distributed over a tracking length of 1000 mm, the positioning of the wire planes and thermal effects were major concerns for the spectrometer design. Fig. 4 shows a front section view of a DC module within the cradle and magnet rail structure (only a few wires shown). A V layer is shown within the circular FR4 (flame resistant G10) gas box, and the coordinate system is indicated.

To position each wire plane and cathode foil as accurately as possible in the z direction, each module layer (including gas box base and lid) contains a set of four high precision ceramic spacers of a Russian material known as Sitall CO-115M [3] (similar to Zerodur [4]). These materials were developed for telescopes and are made from a mixture of glass in two different states: The resultant material has an extremely small coefficient of thermal expansion ($\sim 1 \times 10^{-7}$ (dL/L)/ $^{\circ}$ C)

and can be machined and polished to optical flatness. This, combined with Sitall's good strength (elastic modulus $\sim 5.7 \times 10^{10}$ Pa) allows us to accurately determine each wire plane's z position.

Monte Carlo [5] estimates show that to measure the muon decay parameters with an accuracy of about 2×10^{-4} a systematic error of not more than 2×10^{-4} in reconstructed muon decay positron energy, E_e , and angle, $\cos \theta$, is also required. The energy losses of the muon decay positrons along the z axis of the spectrometer are proportional to $1/\cos \theta$ and do not depend on the (x, y) positions of the stopped muons. This means that the true maximum positron energy, due to a muon decay, from a muon stopped in the target $E_0^{\max} = 52.8$ MeV can be calculated from the equation $E_{\text{meas}}^{\max}(\theta) = E_0^{\max} - k/\cos \theta$ (where k is an energy loss at $\theta = 0$). Therefore an absolute energy calibration of the spectrometer can be defined from the muon decay spectrum itself. However, it is essential that the detector system is very precisely manufactured. Following is an estimate of systematic errors due to manufacturing accuracy. The major source of problems would be a systematic error in our length scales in the u , v , or z directions.

The Monte Carlo study shows that a systematic shift in the location of the U wires in the z direction ΔU_z of $\Delta U_z/U_z^{\text{norm}} = |U_z -$

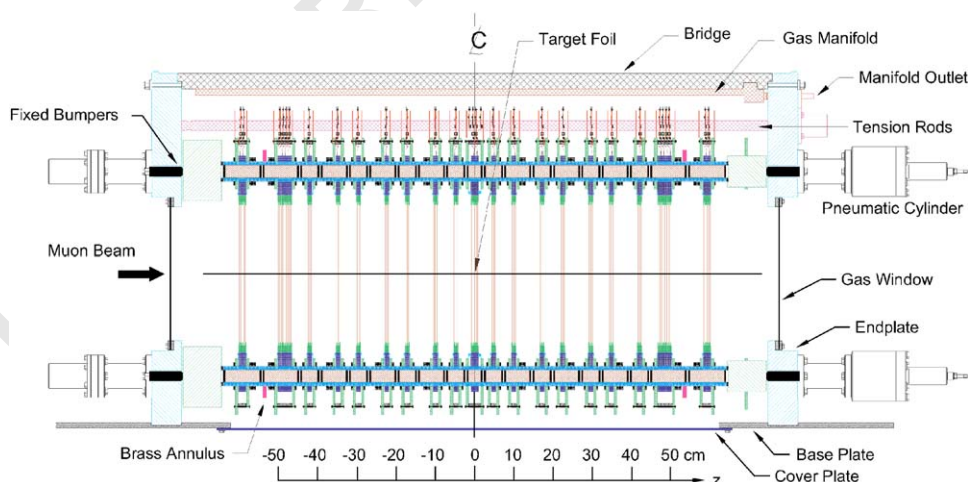


Fig. 3. Side view of the TWIST cradle, showing thick FR4 (flame resistant G10) pieces and stack of 19 modules, all pushed against the upstream cradle endplate by four pneumatic cylinders.

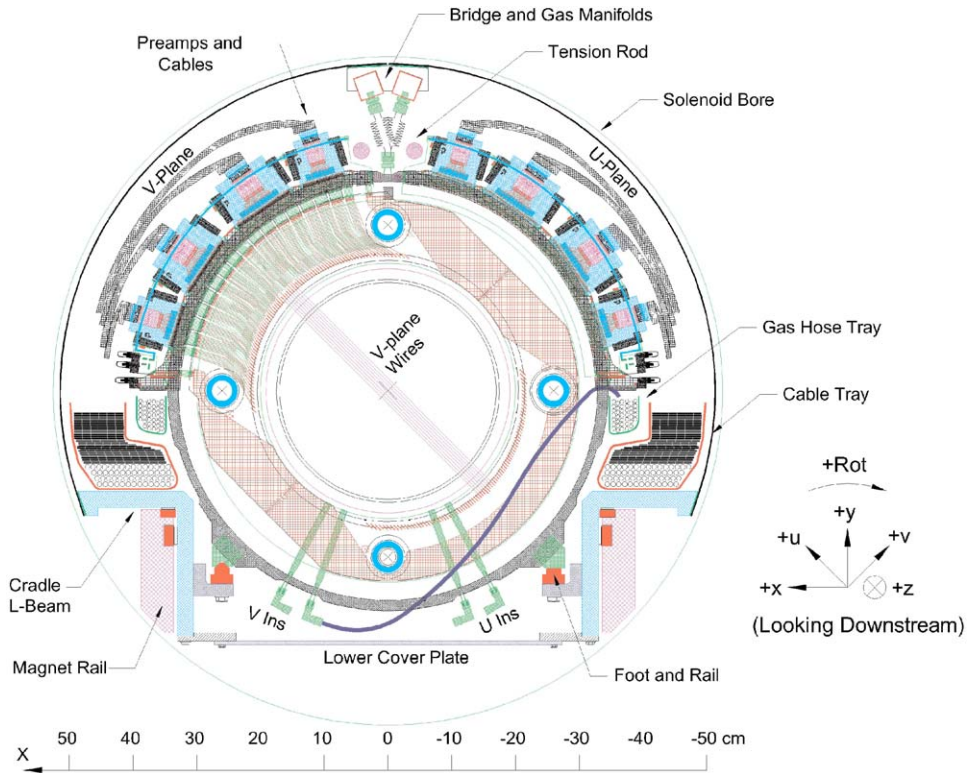


Fig. 4. Front view of DC module in the cradle and magnet rail structure (looking downstream). The coordinate system is indicated.

$U_z^{\text{norm}}/U_z^{\text{norm}} = 5 \times 10^{-4}$ causes a bias in the three muon decay parameters of $|\rho - 0.75| = 1 \times 10^{-4}$, $|\delta - 0.75| = 1.1 \times 10^{-4}$, and $|P_{\mu\xi} - 1| = 6 \times 10^{-5}$. Since we determine the positions of all our wire planes in z to $\sim 30 \mu\text{m}$ (see Sections 6 and 8.3), our error $\Delta U_z/U_z^{\text{norm}} \sim 30 \mu\text{m}/1000 \text{mm} = 3 \times 10^{-5}$ corresponds to a muon decay parameter bias of $\ll 10^{-4}$. Sitall's very small thermal coefficient makes TWIST effectively insensitive (in the z direction) to temperature. Sitall's good strength means that the operating force of 1470 N from a pneumatic cylinder compresses the 1000 mm column of Sitalls (extent of DC modules) by about $24 \mu\text{m}$ (see Section 8). The cylinders have an uncertainty due to their O-ring friction of $\sim 150 \text{N}$, but this corresponds to only $\sim 2.4 \mu\text{m}$, or $\Delta U_z/U_z^{\text{norm}} = 2.4 \mu\text{m}/1000 \text{mm} = 2.4 \times 10^{-6}$.

A systematic shift of $\Delta U_u/U_u^{\text{norm}}$ or $\Delta U_v/U_v^{\text{norm}}$ causes a similar bias in the muon decay parameters. This corresponds to an uncertainty of the

pitch of the wires, or rather, the cumulative uncertainty in wire position across the 320 mm active area of the wire planes. Our wire planes are fabricated on glass substrates (see Section 6 for fabrication details) and surveying of many wire planes indicates that the width of the 320 mm wire plane varies only $\pm 6 \mu\text{m}$ (see Section 3). This variation corresponds to $\Delta U_u/U_u^{\text{norm}} = \Delta U_v/U_v^{\text{norm}} = 6 \mu\text{m}/320 \text{mm} = 1.9 \times 10^{-5}$ which also leads to an insignificant bias in the muon decay parameters. Over 320 mm, the glass plate expands $\sim 1.6 \mu\text{m}/^\circ\text{C}$, so $\Delta U_u/U_u^{\text{norm}}$ and $\Delta U_v/U_v^{\text{norm}}$ are not highly sensitive to temperature.

Monte Carlo studies also showed that the wire positions within each wire plane should be known to less than $20 \mu\text{m}$ RMS. While the positions of the wire planes in (u, v) can be verified, with calibration runs using high energy beam pions, the angles are too small to determine their z positions. It is

clear that the geometry of the TWIST spectrometer exceeds the mechanical tolerances required for this demanding experiment.

3. Chamber design

The layout and the materials of the TWIST drift chambers were chosen to minimize the effect of multiple scattering and energy loss of both the incoming muons and the positrons leaving the target from muon decay. Low mass was also a key requirement of the chambers because the incoming surface muons have a range of only $\sim 140 \text{ mg/cm}^2$ (carbon equivalent). Helium/nitrogen ($\sim 97:03$) flows through the cradle and between the modules, and the first and last cathode foils in each module were also required to act as the module gas windows.

After several GARFIELD [6] studies, and successful prototyping, we chose a simple multi-wire design, where each DC chamber consists of eighty $15 \mu\text{m}$ diameter sense wires at a pitch of 4.0 mm , plus two guard wires on each side. The cathode-to-cathode distance is also 4.0 mm . The cathodes are $6.35 \mu\text{m}$ (nominal) thick doubly aluminized Mylar foil. To keep them as flat as possible, all cathode foils were stretched to a high tension of $>200 \text{ N/m}$ and a high precision gas system was designed, which maintains the differential pressure between the module gases and helium/nitrogen to $\pm 7 \text{ mTorr}$ (see Section 9).

Dimethylether (DME) was chosen as the working gas for DCs. It has some very attractive properties; low Lorentz angle, low atomic number, good resolution and excellent quenching abilities. Due to concerns of wire chamber aging and materials compatibility [7], a long duration aging study was carried out to test all component materials in single-wire test chambers with DME. Suitable materials were found and this damage study has been published [8].

All 44 DCs are identical (fabricated as X layers), but become U or V layers depending on how they are mounted inside the modules. U wires are tilted $+45^\circ$ from vertical, (looking downstream), V wires at -45° . There are seven (UV) modules on either side of the target module and an eight detector-

layer module (VUVUUVUV), designated the dense-stack (DS), at each end of the DC tracking volume. The DC layers start at $|z| = 44 \text{ mm}$ and extend to $|z| = 500 \text{ mm}$.

At the upstream and downstream ends of the stack there are two PC modules with configuration (UVUV). These play a central role in our pattern recognition process. These fast detectors ($\text{CF}_4/\text{isobutane}$) provide discrimination amongst the various tracks that pass through the detector (muon, decay positrons, additional muons and/or decays, beam positrons, delta rays, etc.).

The target module, at the center of the spectrometer, has a somewhat similar (UVUV) configuration, but with the target foil acting as the central cathode. This module plays an important role. The first two detector layers (TG#1 and TG#2) impose fiducial constraints on the (u, v) coordinates of the muon stopping location. These allow us to know that all decays are fully contained within the tracking region. The third TG#3 provides a veto so that any muons that stop past the target foil are eliminated. The muon yields in TG#1 vs. TG#4 (from the tails of the stopping distribution) provide a sensitive estimate of the mean stopping location in the target foil, to a precision of $\sim 10 \mu\text{m}$.

The target and PC modules have a sense-wire pitch of 2 mm . $\text{CF}_4/\text{isobutane}$ was chosen for these modules, since it has high drift velocity and Lorentz angle is not a concern. The target layers extend from $z = -8$ to $+8 \text{ mm}$. The PC layers start at $|z| = 584 \text{ mm}$ and extend to $|z| = 600 \text{ mm}$.

Each wire plane is fabricated on a 3.18 mm thick 60 cm diameter circular glass plate, having a thin printed circuit board (PCB) laminated on the top surface. The four 4 mm thick Sitalls are glued into holes in the glass plate (see Figs. 4 and 5). The wires are strung at the top Sitall surface and a cathode foil sub-assembly positioned at the mid-Sitall point. An extra cathode foil is required to complete each module. This cathode only layer (CO), is also fabricated on a glass plate and uses the same cathode foil sub-assembly.

As mentioned in Section 2, the gas box base and lid also contain a set of four Sitall spacers. The result is that each module layer is in contact at the Sitalls. In the cradle, the modules touch each other

6

R.S. Henderson et al. / Nuclear Instruments and Methods in Physics Research A (2018) 844–854

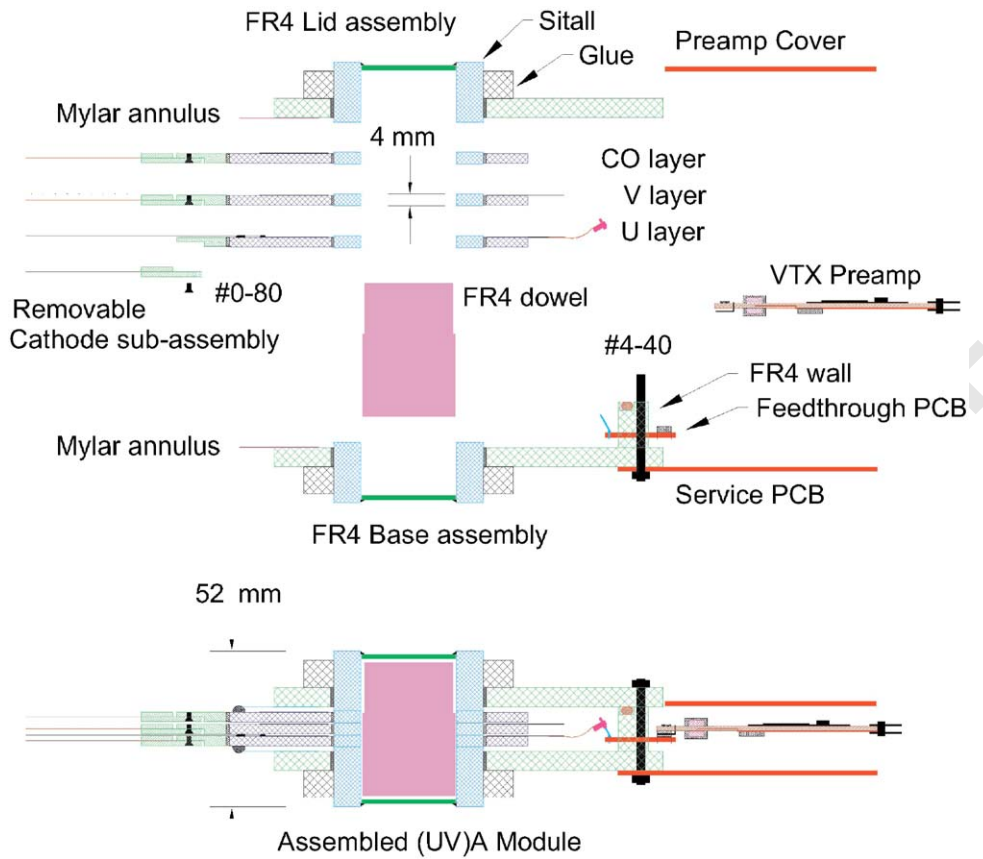


Fig. 5. Section views of the (UV)A module (assembled lower and disassembled upper).

only at their first and last Sitall surface. When the stack of 19 modules is pressed towards the upstream cradle endplate, the force ensures good Sitall-to-Sitall contact (see Section 8).

Our Sitalls typically had surfaces which were flat and parallel to $<0.5\ \mu\text{m}$. Within the thickness groups (4, 8, 20 and 40 mm), the variation in individual Sitall thickness was $\sim 3\ \mu\text{m}$. All Sitall thicknesses were measured and they were arranged in sets of four. Within each set the thickness variation was $<0.5\ \mu\text{m}$. The Sitall thickness data is used to determine the position of each wire plane. In addition, the compression of the Sitalls (in the cradle) frictionally locks each wire plane position in the (u, v) coordinate plane. The actual position of each wire plane is determined by fitting straight tracks from 120 MeV/c pions during calibration runs (see Section 12).

With the wire planes fabricated on glass substrates, the (u, v) positions of wires is less sensitive to temperature (as mentioned in Section 2). With a coefficient of thermal expansion of $\sim 5 \times 10^{-6} (\text{d}L/L)/^\circ\text{C}$, the 320 mm wide wire planes expand $\sim 1.6\ \mu\text{m}/^\circ\text{C}$.

Fig. 4 shows a V layer within the circular FR4 gas box. The 80 sense wire signals pass through the gas box wall to nearby preamps, the output signals travel on mini-coax cables collecting in a cable tray on either side. These cable trays are removable, to allow removal of the cradle and detectors from the seven racks of readout electronics and other services.

The many 0.25" polyethylene gas input lines (one per detector layer) collect in two smaller permanent trays. These gas lines pass between and under the modules to inlet fittings that are

1 accessible when the lower cover plate is removed.
 2 Within the modules, flat polyester “straws” inject
 3 the gas between the detector layers to the active
 4 areas. The module gas outlets are at the top and
 5 connect with soft neoprene bellows to two gas
 6 manifolds, one for DME, the other for CF₄/
 7 isobutane.

8 Each module has two 6.35 mm thick FR4 feet,
 9 one flat and one V-shaped. These feet are doweled
 10 and screwed to the gas box base, they support and
 11 position the modules in the spectrometer by means
 12 of flat and V-shaped rails within the cradle support
 13 structure (see Section 8). Two large longitudinal L-
 14 shaped beams give the cradle great stiffness. The
 15 cradle rolls in and out of the solenoid on the large
 16 magnet rails (see Section 8).

17 During data taking, the 19 modules are im-
 18 mersed in helium/nitrogen (~ 97:03) gas. The
 19 addition of the small amount of nitrogen is
 20 necessary to prevent HV breakdown on the
 21 module exteriors. Each module was tested for
 22 HV breakdown in this gas mixture as part of the
 23 fabrication quality control (QC).

25 4. The (UV)A module

26 **Fig. 5** shows two section views of the (UV)A
 27 module (one disassembled). Section 5 describes the
 28 four other module types (two DC and two PC),
 29 but many of the design features of the (UV)A are
 30 common to all the module types.

31 The (UV)A module consists of five component
 32 layers:

- 33 (1) FR4 gas box base.
- 34 (2) U plane (U).
- 35 (3) V plane (V).
- 36 (4) Cathode-only plane (CO).
- 37 (5) FR4 gas box lid.

39 4.1. Gas box base

40 The gas box base consists of a circular FR4
 41 plate (6.35 mm thick and ~70 cm diameter). This
 42 plate has curved FR4 wall pieces laminated to it,

43 building a full circular wall. In the U and V
 44 readout arcs, the wall contains 1.6 mm thick
 45 feedthrough printed circuit boards (PCBs), which
 46 transfer the 80 sense-wire signals (at HV) from the
 47 detector layer to the two 24-channel and two 16-
 48 channel preamplifiers mounted just outside the
 49 wall. These feedthrough PCBs also bring HV and
 50 pulser signals into the module.

51 A set of four 20 mm long Sitalls is also glued
 52 into holes in the base plate. Since the base and lid
 53 are bolted together at the O-ring seal, we were
 54 concerned that warps in the 6.35 mm thick FR4
 55 plates would result in the gas box warping on final
 56 assembly. To avoid this, bases and lids of gas
 57 boxes are not swapped around, but stay as a pair.
 58 They are bolted together first, then the Sitalls are
 59 glued into the base. Finally, stacks of Sitalls are
 60 added inside the gas box to give the correct
 61 internal distance (12 mm for the (UV) modules).
 62 The Sitalls are then glued into the lid. In this way,
 63 the assembled gas box should have coplanar Sitall
 64 surfaces. Approximately 1 mm inside the outer
 65 surface of these Sitalls, 1.6 mm thick FR4 disks are
 66 permanently glued, making a gas seal. The top
 67 surface of the gas box wall contains an O-ring in a
 68 groove to seal against the gas box lid.

69 An FR4 dowel is inserted into each base Sitall,
 70 forming four posts onto which the other compo-
 71 nent layers are installed. For the (UV)A module,
 72 these four dowels protrude 11 mm into the
 73 module, then narrow and fit more loosely into
 74 the lid plate Sitalls.

75 The Sitall IDs are 32.05 ± 0.05 mm, and the
 76 dowel ODs are 31.93 ± 0.01 mm. If each of the
 77 four Sitalls in each detector layer were positioned
 78 perfectly, this would allow a relative movement of
 79 base, U and V layers of 120 ± 60 μm. In practice
 80 the movement was < 80 μm.

81 The gas box wall also contains two 0.25"
 82 Swagelok gas inlet fittings (one for each wire
 83 plane) and a 0.5" Swagelok fitting for the module
 84 gas outlet. Two 1.6 mm thick service PCBs are
 85 bolted to the gas box base. Each covers ~82° of
 86 arc in the area of the preamps and extend ~60 mm
 87 beyond the gas box wall. These PCBs have preamp
 88 mounting guides, grounding and the preamp
 89 power bus (+4 V).
 90
 91
 92
 93
 94
 95

1 It would have been convenient if the gas box
 2 base (and lid) could have had their own window
 3 foils glued across their central cutouts. Unfortun-
 4 ately, this option was ruled out by considerations
 5 of multiple scattering and the mass budget for the
 6 incoming muons. Instead, a 100 μm thick Mylar
 7 annulus is permanently glued to the inner edge of
 8 these two FR4 plates. These Mylar pieces protrude
 9 40 mm into the central cutout of the FR4 plates,
 10 but stop 4 mm outside the active area. After the
 11 module is assembled, these two Mylar pieces are
 12 glued to the U layer glass plate and CO layer PCB
 13 with latex rubber. This forms a mechanically soft
 14 gas seal and is easily removable. Latex rubber was
 15 chosen, after tests with other synthetic rubbers
 16 (silicones and urethanes) showed extremely high
 17 aging rates with DME ($>1000\%/C$ per cm of
 18 wire) [8].
 19

21 4.2. U plane

23 The U drift plane, as shown in Figs. 4 and 5,
 24 consists of one wire plane and one cathode foil
 25 sub-assembly.

27 This layer has four 4 mm thick Sitalls positioned
 28 accurately and glued into holes in a 3.18 mm thick
 29 60 cm diameter circular glass plate. On the upper
 30 surface of the glass plate, a thin (180 μm) PCB is
 31 laminated. This thin PCB has the solder-pad
 32 pattern for the wires, and traces from the pads to
 33 where flexible output kapton/Cu ribbon cables are
 34 soldered. When the U drift plane is positioned
 35 inside the gas box base (on the FR4 dowels) the
 36 ribbon cables are plugged into connectors on the
 37 gas box feedthrough PCB. No solder connections
 38 are required. Section 6 describes the fabrication of
 39 the wire plane in detail.

41 There is an attached cathode foil sub-assembly
 42 within the central cutout of the glass plate (see
 43 Section 6). Both surfaces of the aluminized Mylar
 44 foil are clamped against copper surfaces and cross-
 45 connected. This foil connection is also brought out
 46 on two kapton/Cu ribbon cables to the gas box
 47 wall PCB.

49 4.3. V plane

51 The V drift plane is identical to the U drift
 52 plane, simply positioned at 90° to the U plane and
 53 on top of it.

55 4.4. Cathode-only plane

57 The cathode-only plane (CO) is similar to wire
 58 plane layers, in that it has four 4 mm Sitalls, a glass
 59 plate and a cathode foil sub-assembly. The PCB is
 60 however far simpler, since there is no wire plane
 61 and only two kapton/Cu ribbon cable connections
 62 of the foil to the gas box wall PCB.

63 With only ~ 0.5 mm between the glass/PCB
 64 layers of the U, V and CO sub-layers, proper
 65 flushing of the two approximately 103 cc active
 66 volumes was a significant design concern. Our
 67 solution was to make flat polyester-film straws,
 68 that directly inject the chamber gas into these
 69 active volumes. These straws have a heat sealed
 70 edge and are permanently glued to the inlet gas
 71 fitting on the inside surface of the gas box wall.
 72 They are 10 mm wide in the flat region and extend
 73 to the active volumes of the U and V plane. During
 74 module assembly, the two straws are easily bent
 75 out of the way, the U plane installed, its straw laid
 76 down on it, then the V plane and its straw, then the
 77 CO plane. This simple and reliable system ensures
 78 good flushing of the active areas of the chambers.
 79

81 4.5. Gas box lid

83 The gas box lid plate is simpler than the gas box
 84 base, with only four 20 mm long Sitalls and the
 85 6.35 mm thick FR4 sheet (with Mylar annulus). As
 86 mentioned in Section 4.1, these Sitalls are glued in
 87 the FR4 lid plate in association with the gas box
 88 base. The lid is bolted down to the gas box base,
 89 forming a gas seal against the O-ring in its groove.
 90 As with the gas box base, there are 1.6 mm thick
 91 FR4 discs glued into the ends of the Sitalls to form
 92 gas seals. After module assembly, a latex rubber
 93 seal is made to the nearest detector layer (the CO).
 94

5. The other four module types

The (UV)A drift module was described in Section 4. There are four other module types in the TWIST spectrometer, they are all based on the same simple structure. They are:

5.1. (UV)B module

This is also a drift chamber module (DC) using DME gas. It is almost identical to the (UV)A module. The only difference is that it has 40 mm long Sitalls in the gas box base instead of 20 mm. By alternating (UV)A and (UV)B modules, for the first seven modules on either side of the target, we produce a better tracking chamber pattern.

5.2. Dense stack

This is also a drift chamber module using DME gas. Like the (UV)B, it has 40 mm Sitalls in the gas box base and 20 mm Sitalls in the gas box lid. However, the wall of the gas box base is approximately three times as tall and, in the two readout regions, has feedthrough PCBs for four wire planes instead of one. Instead of having three detector layers inside the gas box (U,V and CO), the dense stack has nine detector layers (VUVU-VUV and CO). The pattern break in the center is meant to reduce tracking ambiguities. Of course, the FR4 dowels are 24 mm longer as well and there are eight gas inlet fittings and straws instead of two.

5.3. PC module

This module uses four PC wire planes instead of two DC planes. It has a taller gas box wall, with two feedthrough PCBs in each readout area. There are four gas inlets and straws. The five sub-layers in the gas box are UVUV and CO. The Sitalls in the gas box lid and base are all 40 mm long.

The PC wire plane has 160 sense wires, and three guard wires each side, all strung at 2 mm pitch. This gives an active area of 320 mm diameter. The central 32 wires are individually read out to better handle the incoming muon beam and the remainder are read out in groups of four wires, to reduce

the number of readout channels needed. There are 64 readout channels for each PC plane, using four 16-channel preamps. CF₄/isobutane was chosen for the PCs, since it has high drift velocity and the Lorentz angle is not a concern.

5.4. Target module

The target module is the most specialized module in the TWIST spectrometer. The five sub-layers in the gas box are UVUV and CO. Each of the wire planes has its own cathode foil sub-assembly, so there are five cathodes and four wire planes. The major difference of the target module is that the central cathode is also the experimental muon stopping target.

Each target wire plane has 48 sense wires and three guard wires on each side, all strung at 2 mm pitch, and use CF₄/isobutane gas. The 48 sense wires are all individually read out, giving an active area of 96 mm diameter.

This module's main function is to define beam particles entering and exiting the target. Since the axial field confines the low emittance beam particles to small radii, the smaller active area is sufficient.

The major target of interest for TWIST is high purity aluminum of thickness about 70 μm. However, high purity aluminum (>99.999%) foil was not available in the required size. Also, aluminum is far less elastic than Mylar and tests indicated that a foil 340 mm in diameter was not flat enough to act as a wire-plane cathode. A smaller diameter sub-assembly was also not an option, since we wished to keep the mass in this region as low as possible. Therefore, for the initial study of the TWIST spectrometer, the target was 125 μm thick Mylar with carbon [9] on each side (thickness between 5 and 20 μm), for a total of ~145 μm, which has similar stopping power to 70 μm aluminum.

The target foil sub-assembly is fabricated similar to the usual 6.35 μm (nominal) thick aluminized Mylar. The carbon-painted Mylar was stretched and glued between the same two 1.6 mm thick FR4 discs to make a foil sub-assembly. When this sub-assembly is attached to the second U plane, the foil is against the usual FR4 retaining ring, glued into

49
51
53
55
57
59
61
63
65
67
69
71
73
75
77
79
81
83
85
87
89
91
93
95

1 the glass plate (see Section 6). Because of its
 2 greater thickness, this $\sim 145\ \mu\text{m}$ foil is not perfectly
 3 centered between the adjacent V and U wire
 4 planes. For the second U plane, the distance is the
 5 usual $1997\ \mu\text{m}$ (2 mm minus half the foil thickness)
 6 and the wire plane is symmetrically placed between
 7 the adjacent cathode foils. However, for the first V
 8 plane, the wire plane to target foil distance is
 9 $\sim 139\ \mu\text{m}$ less than usual and the wire plane is
 10 effectively off-center. Since these wire planes are
 11 not used for precision tracking, this was accep-
 12 table.

13 While the Mylar target was in use, we developed
 14 a new technique for the aluminum target foil. This
 15 uses a stretched Mylar foil with a central cutout. A
 16 small diameter aluminum foil is then glued over
 17 this hole. The Mylar is $25\ \mu\text{m}$ thick doubly
 18 aluminized, with a 120 mm diameter hole, and
 19 effectively acts as a spring to keep the aluminum
 20 foil tensioned and flat. The aluminum foil is
 21 150 mm in diameter, so there is a 15 mm overlap
 22 glue region. TRA-CON conductive silver epoxy is
 23 used to ensure electrical connection to the Mylar
 24 foil. The aluminum foil is $71 \pm 1\ \mu\text{m}$ thick and the
 25 purity is $>99.999\%$ [10]. To avoid any problems
 26 with this glue region, we also inserted a pair of
 27 $25\ \mu\text{m}$ thick kapton masks in each of the wire
 28 planes adjacent the target foil. These masks
 29 eliminate gas gain elsewhere and have a central
 30 cutout 110 mm in diameter. Only the central
 31 region of the target planes is of interest (their
 32 active width is only 96 mm), so these masks do not
 33 affect the target module performance.

34 The end result is a target module with a well-
 35 tensioned high purity central aluminum target foil
 36 and an active area of about 100 mm diameter; but
 37 still having low mass out to 330 mm diameter. The
 38 resultant combination foil has worked very well.
 39 By choosing which side of the Mylar the aluminum
 40 foil is glued on, and using $39\ \mu\text{m}$ thick spacers, we
 41 were able to position the center of the aluminum
 42 foil mid-way between the V and U wire planes.
 43 Now both these wire planes are closer to the target
 44 foil than their other foil, but the difference is only
 45 $32\ \mu\text{m}$ instead of the $139\ \mu\text{m}$ for the earlier Mylar/
 46 carbon target.
 47

5.5. Mirror modules

51 The aim of the TWIST spectrometer is to be as
 52 symmetric as possible with respect to the central
 53 target foil. We therefore decided that the nine
 54 modules on either side of the target module should
 55 be mechanically mirrored, i.e., they should all have
 56 their gas box lid plates facing the central target.

57 With this in mind, the gas boxes were designed
 58 with removable feet. These feet, one flat and one
 59 V-grooved, position the module in the cradle. By
 60 switching the feet, and rotating about the vertical
 61 axis, a gas box can be used in either position. This
 62 effectively reduces the different module types from
 63 nine to five. However, rotating a module like this
 64 effectively turns a U plane into a V plane, and vice
 65 versa, introducing an asymmetry. Therefore, while
 66 the components are the same, a module is
 67 assembled differently if it is to be used in the
 68 upstream or downstream half of the spectrometer.
 69 For example, a downstream UV module has the
 70 first wire plane installed in the module gas box
 71 tilted $+45^\circ$ (looking into the open gas box). So a
 72 downstream (UV) is assembled (Base, $+45$, -45 ,
 73 CO, Lid), while an upstream (UV) is assembled
 74 (Base, -45 , $+45$, CO, Lid).
 75

5.6. Spare modules

76 We also produced five fully instrumented spare
 77 modules, one of each type; (UV)A, (UV)B, dense
 78 stack, target and PC. In the two years since the
 79 TWIST spectrometer was commissioned, the
 80 performance of the TWIST modules has been
 81 excellent. All 3520 DC wires operated at full
 82 efficiency with no dead or hot wires. One PC wire
 83 broke at the end of a long period of data taking,
 84 thereby requiring the module to be removed and
 85 replaced with the spare PC module. The damaged
 86 PC module was repaired and is now the spare. The
 87 second target module allowed the aluminum target
 88 to be installed and the module to be fully tested,
 89 ready for a quick replacement in the spectrometer.
 90
 91
 92
 93

49

51

53

55

57

59

61

63

65

67

69

71

73

75

77

79

81

83

85

87

89

91

93

95

6. Wire plane fabrication

As mentioned in Section 3, a TWIST wire plane layer, consists of one wire plane and one removable cathode foil sub-assembly. The wire plane design is based on a 3.18 mm thick circular glass plate. This plate has a diameter of ~ 600 mm, with a central cutout of ~ 398 mm diameter and four smaller ~ 54 mm diameter holes positioned every 90° and 260 mm from the center.

The steps to fabricating a wire plane are as follows:

- (1) Glue thin PCB ($180\ \mu\text{m}$) on a glass plate.
- (2) Glue set of four 4 mm Sitalls into glass plate.
- (3) Glue FR4 cathode retaining ring into central cutout of glass plate.
- (4) String wires above PCB surface.
- (5) Glue wires to glass plate (glue bumps), rotate winding table to vertical, allow to set overnight.
- (6) Rotate winding table to horizontal, solder wires to PCB. Trim and clean.
- (7) Measure wire tensions, replace if $T < 26$ g.
- (8) Put wire plane on milling machine. Mill glue and solder bumps to $\leq 650\ \mu\text{m}$ from glass.
- (9) Measure wire positions in x and z .
- (10) Replace wires out of position $> 20\ \mu\text{m}$ in x .
- (11) Solder 19 flexible kapton/Cu ribbon cables on readout edge of PCB.
- (12) Clean and store until module assembly.
- (13) Install cathode foil sub-assembly with #0–80 nylon screws.

The removable cathode foil sub-assembly is fabricated by stretching the $6\ \mu\text{m}$ foil, then gluing it to a 1.6 mm thick FR4 annulus (ID = 339 mm, OD = 379 mm). When the glue sets, two small dowel holes are cleaned and the Mylar pierced, then a second 1.6 mm thick FR4 annulus (ID = 339 mm, OD = 360 mm) is doweled and glued to the other side of the Mylar. When trimmed and cleaned, the resultant assembly is reasonably flat. The foil sub-assembly is attached to the cathode retaining ring by 24 #0–80 nylon screws. The difference in ODs means that the foil surface is clamped against the retaining ring, making the foil z position insensitive to the

thickness of the FR4. Two “notches” in the larger FR4 annulus allow both sides of the aluminized Mylar to be clamped against copper surfaces, ensuring reliable low impedance connections to the thin PCB laminated on the glass plate. Two flexible kapton/Cu cables bring these ground connections to the gas box wall feedthrough PCB.

Although the wire planes are mounted as U or V planes in the modules, during fabrication, they are considered as X planes (wires vertical). For step (2), the set of four Sitalls are clamped on a thick glass assembly table which is flat to $\pm 0.5\ \mu\text{m}$. For step (3), the incomplete unit is again clamped on the assembly table (only at the Sitalls), the FR4 retaining ring is positioned on glass spacers in the cutout and glued in place. While the wires are strung at the surface height of the 4 mm Sitalls, the cathode foil retaining ring is positioned as accurately as possible 2 mm away, at the mid-thickness.

During stringing, the detector layer is clamped down (only at the Sitalls) to a similar thick flat glass winding table. The wire plane is strung using precision glass combs. Stringing was carried out manually, in a class 1000 clean room. The room temperature was held stable within $\pm 1^\circ\text{C}$. When positioned from comb-to-comb, the wire is above the PCB surface, so the height of the wires (z position) is set by the glass combs and is therefore precise relative to the Sitall surfaces.

All wire chambers use $15\ \mu\text{m}$ diameter gold-plated tungsten/rhenium W(Re) sense wires. Lengths of wires vary from 40 cm in the center of a plane to 23 cm on the edge. As each wire is strung, one end is soldered to an external pad, then it passes across the two glass combs, and is then tensioned and soldered to another external pad. When the full plane of wires is strung in this way, each wire is glued to the glass plate (just beyond the cutout) with small epoxy glue beads. When this is completed for the whole plane, the winding table is rotated to the vertical position and the glue is allowed to set overnight. In this way, the wire plane is strung horizontally, but finally moved to the vertical, so that gravitational sags of the glass plate do not affect wire positions in z . This matches how the wire planes are positioned in the TWIST experiment. The next day, the winding

1 table is rotated back to the horizontal, the wires
2 soldered to the PCB pads and trimmed.

3 With only ~ 0.5 mm between the glass/PCB
4 pieces of the detector layers, the height of the wire
5 solder bumps and glue beads was a problem.
6 Attempts to keep them shallow were a failure and
7 several glass plates were broken in early prototype
8 modules. Our solution was to place the wound
9 wire plane in a milling machine (mounted at the
10 Sitalls), and machine any solder and glue surfaces
11 that were too high. In this way we guaranteed a
12 clearance of ≥ 0.15 mm.

13 All drift chamber layers (DCs) are the same,
14 having 80 sense wires, plus 2 guard wires on each
15 side, with a pitch of 4.0 mm. The PC wire plane,
16 has 160 sense wires, and an active area of 320 mm
17 diameter. The target wire plane has 48 sense wires,
18 and an active area of 96 mm diameter. The PC and
19 target planes both have three guard wires on each
20 side and a wire pitch of 2.0 mm. All three wire
21 plane types are wound on the same winding table
22 and with the same procedure.

23 The fully instrumented spectrometer has 19
24 modules and required 44 DC planes, four target
25 planes, eight PC planes and 19 CO planes. The five
26 spare modules contain another 12 DC planes, four
27 target planes, four PC planes and five CO planes.

28 Quality control was carried out during all steps
29 of fabrication. This was essential to ensure
30 reproducible results during the production. The
31 mechanical parameters of every detector layer
32 (dimensions of components, wire tensions and
33 positions, etc.) were measured during production
34 and stored in a data base.

35 For electrostatic stability at 2000 V, only a 4 g
36 tension is theoretically required for 40 cm long
37 $15\ \mu\text{m}$ diameter tungsten wires. We used 35 g
38 weights, well below the ~ 50 g typical breaking
39 tension of $15\ \mu\text{m}$ W(Re).

40 Average measured wire tensions are about 31 g,
41 the difference being due to the friction of wires on
42 the winding equipment. The distribution of
43 measured tensions for all 6,784 sense wires on all
44 56 DC, 12 PC and 8 target layers had an RMS of
45 only 1.25 g. All wires with tension less than 26 g
46 were replaced.

47 After stringing, machining of the solder and glue
48 bumps, and tension measurement, the position of

49 each wire in the plane is mapped. This is usually
50 only done in the plane of the wires, i.e., the x value
51 for two well separated values of y (along the wire).
52 However, since we were going to so much effort to
53 control the z positions, with glass surfaces and
54 glass combs, etc., we also wanted to measure the z
55 position of each wire (at two values of y).

56 This mapping in x and z was achieved using a
57 digital readout carriage with two CCD cameras.
58 One camera observed the wire from directly above
59 the plane. The carriage was moved until the wire
60 was centered on a monitor with cross-hairs and the
61 digital scale readout gave x directly. To measure
62 the z coordinate, a second camera was mounted to
63 view the wire from a 45° angle. Using a second
64 monitor and cross-hairs, the difference in the two
65 values of the digital readout gave the z position.
66 So, the (x, z) wire positions on each wire were
67 measured at two values of y , 20 cm apart.

68 Fig. 6 shows wire x position residuals (distance
69 from correct location) for a typical DC wire plane,
70 plus the distribution of those x residuals. Two
71 measurements were made of this wire plane, by
72 different operators, eight months apart. The first
73 measurement was done immediately after winding.
74 The second was made after replacement of wire
75 number 18 (shown as a star). This figure shows the
76 excellent reproducibility of the measured wire
77 positions and also of the wire replacement
78 ($< 3\ \mu\text{m}$). Tests on a glass ruler with precise
79 diamond cut grooves indicate the measurement
80 accuracy is $\sim 2.3\ \mu\text{m}$ for x .

81 Fig. 7 shows the distribution of measured x wire
82 position residuals summed for 6,304 wires (from
83 50 DC planes, 12 PC and 8 target layers), with
84 $\sigma = 3.3\ \mu\text{m}$. These residuals were from the readout
85 side of the wire plane; similar results were obtained
86 on the nonreadout side (20 cm away in y). A total
87 of 77 wire planes were fabricated (including those
88 in the spare modules), having 6,944 wires. Our
89 database contains all measured (x, z) values.

90 For the 77 wire planes, there are very few wires
91 out of position more than $15\ \mu\text{m}$ in x . As part of
92 our QC, we replaced any wire more than $20\ \mu\text{m}$ out
93 of position. Only three were missed, all less than
94 $25\ \mu\text{m}$. The results demonstrate that our winding
95 equipment has provided high quality wire plane

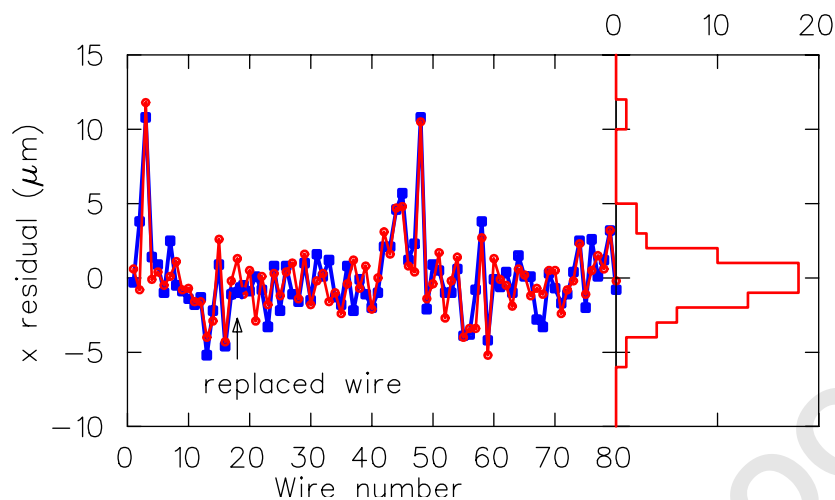


Fig. 6. Wire x position residuals (distance from correct location) for a typical DC wire plane. Blue squares are measurements soon after fabrication, red circles are data remeasured 8 months later.

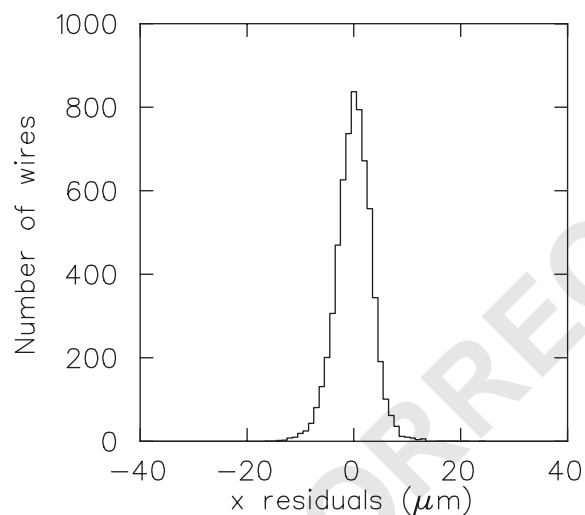


Fig. 7. Wire x position residuals summed for 6,304 sense wires from the readout side of 70 wire planes (50 DC, 12 PCs and 8 target planes), with $\sigma = 3.3 \mu\text{m}$.

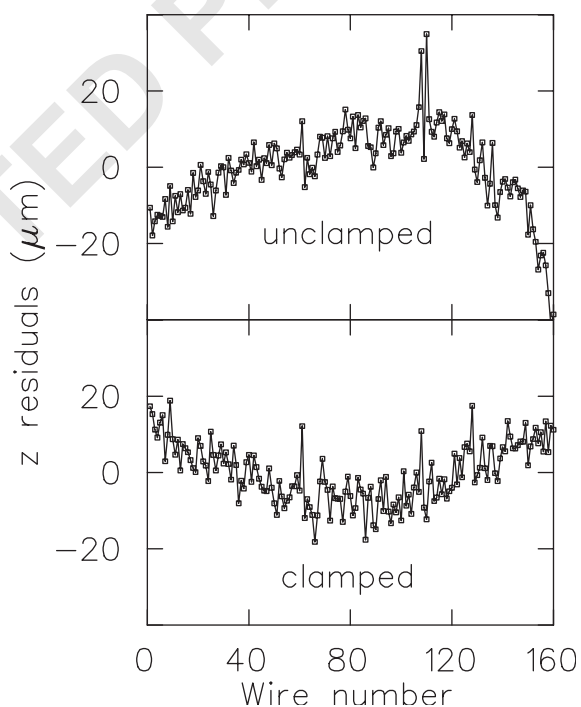


Fig. 8. Wire position z residuals for PC wire plane (#153) without clamping (upper) and with clamping (lower).

production, despite using many people over a two year production period.

Similarly, Fig. 8 shows the wire position residuals for a typical PC plane in the z direction (negative being down). The upper part shows the results for the plane unclamped, the lower part the same wire plane clamped. By clamped, we mean there was force applied to each Sitall, pushing it

down against the granite surface of the scanning table. The change is significant. One can see that while the wire-to-wire variation is similar to the x

1 measurement, the range of the z residuals is much
 2 larger, $\sim 60\ \mu\text{m}$ (for unclamped) compared to
 3 $\sim 19\ \mu\text{m}$ for the x residuals of Fig. 6.

4 This is understood as follows. During the final
 5 stage of stringing (when the glue beads are setting)
 6 the wire plane was vertical and bolted firmly (at
 7 the Sitalls) to a solid and flat glass plate. However,
 8 during the (x, z) wire position mapping, the wire
 9 plane was horizontal and not clamped down. It
 10 was therefore subject to flexing and gravitational
 11 sag. The calculated gravitational sag of the glass
 12 plates (midway between Sitalls) is $17\ \mu\text{m}$. But we
 13 see in the upper part of Fig. 8, that this unclamped
 14 wire plane is not sagging down, but flexing up. The
 15 maximum bending of the glass plates due to wire
 16 tension loads was calculated using ANSYS [11] to
 17 be only $1.3\ \mu\text{m}$ for a DC plane and $2.6\ \mu\text{m}$ for a PC
 18 plane, this is not significant.

19 It was found that, because the glass plates were
 20 slightly warped, there had been concern that they
 21 would touch each other, since the gaps between
 22 detector layers are only $\sim 0.5\ \text{mm}$. To avoid this,
 23 weights had been placed on the glass plates during
 24 their gluing to their set of Sitalls (step (2) in list).
 25 Naturally, when released, they sprang back to
 26 their natural shape. During gluing of the cathode
 27 retaining rings and stringing, the planes were again
 28 clamped to the assembly and winding tables,
 29 respectively, but during (x, z) measurement they
 30 were unfortunately not clamped.

31 Fig. 8 demonstrates that, when the same wire
 32 plane was clamped, the glass plate was forced
 33 much flatter again (lower part of figure). It now
 34 shows the center of the wire plane $\sim 18\ \mu\text{m}$ lower
 35 than the edges, in good agreement with the
 36 calculated gravitational sag of $17\ \mu\text{m}$. Unfortun-
 37 ately, this wire plane was the only one not in the
 38 experiment or in spare modules, so other clamped
 39 z residual data could not be obtained.

40 Tests indicate that a load of only $50\ \text{N}$ is
 41 required on each Sitall to clamp the glass plate
 42 to its flattened state. In the cradle, the Sitall
 43 columns are compressed with $1470\ \text{N}$, so we
 44 believe all the wire planes are certainly flattened.
 45 Also, since the planes are vertical, the $17\ \mu\text{m}$
 46 gravitational sag should not be present. Our
 47 existing z maps allow us to determine if any wire
 is out of z position by more than $\sim 10\ \mu\text{m}$ (relative

49 to its neighbors). As part of our QC we replaced
 50 any wire that was out of z position by more than
 51 $\sim 25\ \mu\text{m}$ (relative to its neighbors). Only four wires
 52 out of position by more than $50\ \mu\text{m}$ in z were
 53 missed.

54 Few of our 77 wire planes are badly warped in z .
 55 The wire plane shown in Fig. 8 is among the worst.
 56 Most have warps $< 20\ \mu\text{m}$. The summed data of z
 57 residuals has $\sigma = 8.4\ \mu\text{m}$. This is quite low,
 58 considering that even a clamped wire plane has a
 59 gravitational sag of $17\ \mu\text{m}$ (calculated).

60 7. Bench tests

61 All modules were bench tested before use in the
 62 TWIST spectrometer. Gas gain was measured
 63 across each wire plane using an argon/isobutane
 64 (25:75) gas mixture and ^{55}Fe X-rays. This mixture
 65 has an operating voltage similar to that of DME.

66 These tests showed that signal pulse height
 67 uniformity is within 20%. The variation is mostly
 68 due to increase of anode-cathode gaps in the
 69 centers of planes because the outer cathode foils
 70 also serve as gas windows and differential pressure
 71 between chamber gas and environment was not
 72 perfectly zeroed for these tests. Another test was
 73 carried out with a $10\ \text{mCi}$ uncollimated ^{90}Sr source
 74 in order to check the ability of each plane to hold
 75 high voltage with current up to $50\ \mu\text{A}$ for at least
 76 30 s.

77 Modules were also tested for gas tightness with
 78 helium. For (UV), target, and PC modules, a leak
 79 rate less than $< 0.3\ \text{cc}/\text{min}$ was considered accep-
 80 table. For the dense stack modules, leak rates
 81 $< 0.6\ \text{cc}/\text{min}$ were accepted (see Section 9.3 for
 82 details).

83 Modules were also tested for HV stability in
 84 helium/nitrogen (97:03). This was done with pure
 85 isobutane in the module to over-quench them and
 86 allow testing at higher than operating voltage. All
 87 assembled modules have passed these bench tests.

88 8. Module support—the cradle

89 The TWIST solenoid has a bore diameter of
 90 $1050\ \text{mm}$. To position the nineteen TWIST detec-

tor modules, the cradle was designed to be as rigid as possible, so the positions of wires (in x, y, z) are well understood and constant during long periods of data taking. As was seen in Fig. 4 (the front view of DC module in cradle structure), the L-shaped cradle beams and the magnet rails were made as large as possible while allowing the entire structure to be moved up to 10 mm (in any direction) within the solenoid bore. The cradle and magnet rails are made of aluminum (6061 T6). All screws, bolts and dowels are of non-magnetic titanium or brass.

Fig. 9 shows a 3d drawing of the cradle and magnet rail structure (not true colors). The two magnet rails are $5\text{ cm} \times 18\text{ cm}$ and 265 cm long. The downstream ends of the rails come almost to the magnet door. When the magnet door is open, an external cart having similar profile beams can be connected to the magnet rails to allow the cradle to roll in or out of the magnet. Seven racks of services associated with the cradle are mounted on a rolling platform. As the cradle is rolled out, this platform is rolled downstream. These services

include the HV supplies, postamp/discriminators, +4 V preamp supplies, and the gas system.

The main components of the cradle are the two longitudinal beams, the two endplates, the “bridge” and the tension rods. The beams have an L shape, with the vertical part being 23 cm high and the horizontal part 18 cm wide, and both arms are 2.5 cm thick. On the inside face of each beam, there is a module support rail. As Fig. 4 showed, one of these module rails is V shaped, the other is flat. The insulating feet on the modules (FR4) match these profiles and position each module in the cradle in the (x, y) plane (or (u, v)). The cradle beams continue 27 cm beyond the endplates. Four sets of Be/Cu roller bearings, under the ends of the beams, allow the cradle to roll on the magnet rails during installation or removal. During the final few inches of installation, four 2.54 cm diameter titanium dowels (rounded tips) on the cradle begin to engage dowel holes and horizontal slots in aluminum blocks mounted on the magnet rails. With a dowel hole and precision slot at each end of the cradle, it can be reinstalled with an (x, y)

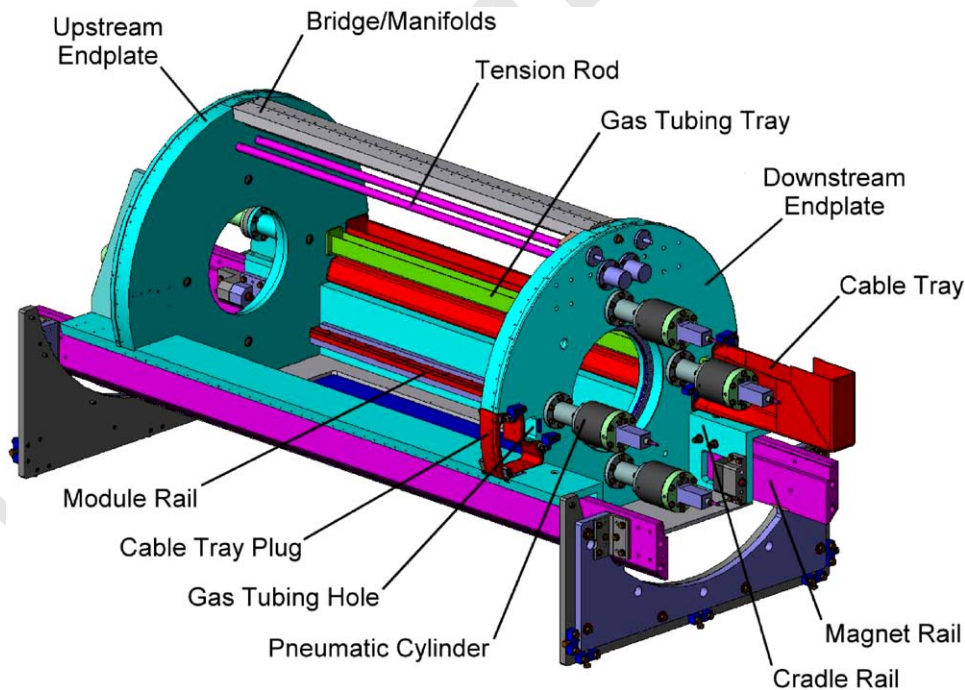


Fig. 9. Cradle and magnet rail structure for the TWIST modules. One cable tray and gas tray are removed.

1 reproducibility of ≤ 0.1 mm, which was as good as
 2 the measurement technique used. These dowels
 3 and blocks lift the cradle ~ 0.3 mm, so there is no
 4 mechanical conflict with the rollers and they are
 5 not under continuous load. The z location of the
 6 cradle is ensured by having two mating surfaces at
 7 the downstream end.

8 The two cradle endplates are 76 mm thick
 9 aluminum (6061 T6). Each has a central cutout
 10 and step for a window assembly (O-ring sealed),
 11 the windows being 25 μ m doubly aluminized
 12 Mylar and positioned 2.8 cm from the inside
 13 endplate face. The endplates are doweled, bolted
 14 and glued to the cradle rails. As discussed in
 15 Section 3, the accurate positioning of the wire
 16 planes in the z direction relies on compressing the
 17 four columns of Sitalls coming from the nineteen
 18 modules. There are 113 Sitalls in each column and
 19 they are compressed towards the upstream direc-
 20 tion by four custom pneumatic cylinders mounted
 21 on the downstream endplate. These aluminum
 22 cylinders each have a cross-sectional area of
 23 42.7 cm² and a maximum operating pressure of
 24 100 psi. We operate them at 50 psi, where they each
 25 compress the Sitall columns against the upstream
 26 endplate with a force of 1470 N. The gas used in
 27 the cylinders is helium rather than air, so that any
 28 small gas leaks do not contaminate the cradle gas.

29 To further stiffen the upstream endplate against
 30 this 5880 N load, there are two 51 cm \times 25 cm \times
 31 2 cm struts between this endplate and the L beams.
 32 Since the cradle beams are at the bottom of the
 33 cradle, there would still be a tendency for the
 34 endplates to separate at their top edges. To prevent
 35 this, the cradle also has two 2.5 cm diameter
 36 aluminum tension rods at the top. These rods are
 37 removed when modules are added or taken from
 38 the cradle. The tension rod design ensures the
 39 lengths are reproducible, so the upstream end-
 40 plate's position and shape do not change.

41 As can be seen in Fig. 9, the downstream
 42 endplate has a pair of openings on each side. One
 43 is a simple cutout (approximately 34 cm²) just
 44 outside the cylinders at $x = \pm 260$ mm ($y = 0$).
 45 They are for two permanent trays that hold a total
 46 of sixty 0.25" polyethylene gas inlet lines, 56 for
 47 the detector layers plus four spares. These trays
 and gas lines are permanently installed and sealed

49 with silicone glue as they pass through the down-
 50 stream endplate. If the cradle is removed from the
 51 area, these gas lines are easily disconnected from a
 52 nearby external panel and the short hoses taken
 53 with the cradle. The bottom of the cradle has a
 54 12.7 mm aluminum plate bolted and glued in place.
 55 This plate has a 124 cm \times 48 cm cutout and a set of
 56 blind tapped holes for a removable O-ring sealed
 57 bottom cover plate. This 6.4 mm bottom cover
 58 plate gives access to the bottom of the cradle
 59 (when it is out of the magnet) to connect or
 60 disconnect input gas lines from the modules.

61 The other pair of openings on the downstream
 62 endplate have much larger cutouts (approximately
 63 175 cm² each) and are designed for cable trays
 64 containing the module output mini-coax cables,
 65 the preamp LV cables, the HV cables, module gas
 66 and cradle gas temperature probe cables, and two
 67 NMR cables used for field probes. If the cradle
 68 was to be removed from the area, we decided we
 69 wanted to open the cradle and unplug cables from
 70 the preamps, etc., then leave these two cable trays
 71 behind. The alternative was to disconnect all these
 72 many cables from the readout electronics, HV
 73 supplies, etc., then coil these long cables back to
 74 the cradle and remove them with it. In particular,
 75 the ~ 5000 signal mini-coax cables (plus spares)
 were deemed too fragile for this process.

77 In order to leave these cable trays behind, two
 78 removable gas seals were required at the down-
 79 stream endplate. Our solution was to make a
 80 curved and tapered 76 mm thick aluminum plug
 81 that surrounded a short section of the cable tray
 82 and could mate with an appropriately shaped
 83 cutout in the downstream endplate. A 3.2 mm
 84 thick Poron rubber gasket, between the plug and
 85 cutout, is compressed to ~ 2.0 mm during its
 installation forming a good gas seal.

87 The tray was screwed and glued to the plug,
 88 then the cables were sealed within the tray with
 89 silicone rubber. The latter was difficult with so
 90 many cables; air leaks around and through these
 91 cables dominate the cradle leakage. The cradle air
 92 leak rate of ~ 2.5 cc/min is quite acceptable and
 93 only results in the cradle gas containing $\sim 0.03\%$
 94 air. The cradle has been removed and installed
 95 several times. The removable cable tray design has
 shown itself to be simple and reliable.

The “bridge” is a removable aluminum structure that is positioned at the top of the cradle above the modules and tension rods. It holds the two outlet gas manifolds (see Fig. 4 and Section 9). The sixteen DC modules are connected to one manifold, the target and two PC modules to the other. The connections are via soft neoprene rubber bellows, so little or no force is applied to the modules. The last and major gas seal of the cradle is made by two 2.4 mm thick aluminum shells that have gasket seals (Poron) to the bridge, the endplates and the outside edge of the cradle L-beams. Each of the shells cover an angle range of approximately 103° on each side of the cradle.

8.1. The 100 mm thick upstream FR4 annulus

Unfortunately, one cannot simply push the most upstream module against the cradle upstream endplate. The endplate is aluminum and the modules are glass and FR4. They have thermal expansion coefficients of 2.7×10^{-5} , $\sim 0.5 \times 10^{-5}$ and $\sim 1 \times 10^{-5} (dL/L)/^\circ\text{C}$, respectively. The Sitalls are at $x = \pm 260 \text{ mm}$ ($y = 0$) and $y = \pm 260 \text{ mm}$ ($x = 0$). So, over 520 mm the differential thermal expansion is $> 11 \text{ mm}/^\circ\text{C}$. For a 10°C change, the massive 76 mm thick endplate would be trying to stretch the module $> 110 \mu\text{m}$. This was considered too dangerous. In addition, pushing the brittle Sitalls against the aluminum plate was deemed unwise. As a final concern, the endplate could not be guaranteed flat enough or stiff enough.

Our solution was to use a 100 mm thick annulus of FR4 upstream of the first module. This FR4 annulus has OD of 680 mm and an ID 340 mm, with four holes milled through it, at $x = \pm 260 \text{ mm}$ ($y = 0$) and $y = \pm 260 \text{ mm}$ ($x = 0$). These four holes each have a larger diameter step in the upstream face. Four 40 mm long Sitalls are glued into the downstream face, using the same optically flat assembly table used for the detector layers. The holes in the Sitalls are sealed with 1.6 mm thick FR4 discs and the holes in the FR4 annulus are filled with a mixture of epoxy and fine sand. Finally, 19 mm thick hard brass inserts (naval brass) are glued and screwed to the upstream face of the annulus.

This system creates a coplanar set of Sitalls for the upstream module to be pushed against, and transfers the four 1470 N loads to the annulus. Because the FR4 has a thermal coefficient close to glass, the module should not be stressed. Being 100 mm thick, it is very rigid. The sand-filled epoxy creates a smooth load transition to the FR4 and has less compression than regular epoxy. Contact to the brass inserts is made with four 25 mm diameter rounded aluminum bumpers that are mounted on the outside of the upstream endplate and protrude into the cradle. Their z position is adjustable and lockable. The threaded region is 22 cm from the inside surface of the cradle. This distance allows the bumpers to flex slightly in the (x, y) plane, to minimize the effects of the different thermal coefficient of FR4 and the aluminum endplate. The FR4 annulus has suitable feet machined into it, for the V shaped and flat rails inside the cradle.

8.2. The downstream FR4 piece

At the downstream end of the cradle, the situation is quite different. It is still important to provide a transition for the four 1470 N loads from the pneumatic cylinders to the brittle Sitalls. The issue of differential thermal coefficients is also the same as for the upstream end of the cradle. However, while great stiffness of the upstream annulus was an asset, at the downstream end of the cradle, compliance is desired. The reason is obvious; we want the four 1470 N loads transferred to the downstream module’s Sitalls. A stiff annulus, if its four Sitalls were not perfectly coplanar, might not transfer those four loads evenly.

Our solution is to have four 80 mm diameter, 100 mm thick FR4 rods mounted on a 6.4 mm thick FR4 annulus. Each of these FR4 rods has a through hole, with a 40 mm long Sitall, and brass insert glued into it, just like those of the upstream annulus. These four 80 mm diameter FR4 rods provide the force transitions; the 6.4 mm thick FR4 annulus supports them, but is quite flexible. The pneumatic cylinders, mounted on the downstream side of the endplate, each have a 25 mm

1 diameter rounded aluminum bumper attached to
2 its piston.


3 These bumpers protrude into the cradle. This
4 distance from the brass insert to the piston allows
5 the bumpers to flex slightly in the (x, y) plane,
6 minimizing the effects of the different thermal
7 coefficient of FR4 and the aluminum endplate.
8 The 6.4 mm thick FR4 annulus has suitable feet
9 machined into it, for the V-shaped and flat rails
10 inside the cradle.

11 8.3. Compression of the 19 modules

12 The stack of 19 modules is compressed by the
13 four pneumatic cylinders. At their maximum
14 pressure of 100 PSI, each of these cylinders pushes
15 its Sitall column with a force of 2940 N.
16 Compression tests were performed to check that
17 we understand what this compression of the
18 modules is actually doing.

19 With such tests in mind, the pneumatic cylinders
20 were designed with the shaft protruding from both
21 ends of the cylinder. In this way, dial gauges could
22 be mounted outside the cradle to measure the
23 movement of the cylinders. Unfortunately, since
24 the gauges have to be mounted on the cylinder
25 casing, their measurements also include movement
26 of the cradle endplates (especially the downstream
27 endplate). This cradle movement is about eight
28 times larger than the compression of the Sitalls
29 (see top curve in upper part of Fig. 10). To
30 subtract the effect of the movement of the cradle,
31 we substituted four aluminum pipes for the
32 detector stack. The response was approximately
33 linear, especially for $f > 1100$ N. This data was
34 corrected for the expected compression of the
35 pipes ($1.46 \times 10^{-3} \mu\text{m}/\text{N}$) and used as the deflection
36 characteristic of the cradle (see bottom curve
37 in upper part of Fig. 10). The lower curve in Fig.
38 10 shows the compression tests of the module
39 stack, after subtraction of the cradle deflection.

40 As can be seen, the stack of 19 modules shows
41 an initial large compression, which becomes linear
42 for $f > 1400$ N. This response is understandable;
43 the modules have to be pushed into contact and
44 then the increased force hopefully drives them into
45 nearly optical contact of their flat surfaces. After
46 optical contact, the expected slope of the data

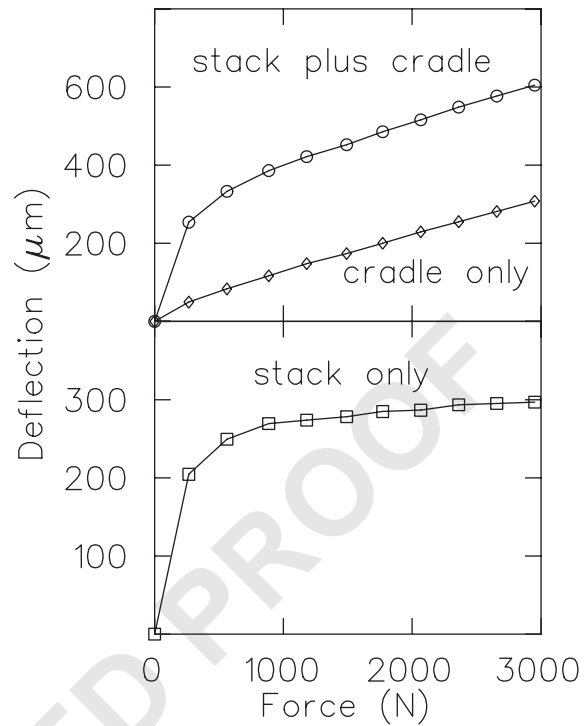

49
50
51
52
53
54
55
56
57
58
59
60
61
62
63
64
65
66
67
68
69
70
71
72
73
74
75
76
77
78
79
80
81
82
83
84
85
86
87
88
89
90
91
92
93
94
95

Fig. 10. Compression of module stack by pneumatic cylinders. The upper part shows plots of responses for the cradle as well as for the module stack plus cradle. The lower plot shows the derived stack response.

should be determined by the elastic modulus of the Sitall ($\sim 5.7 \times 10^{10}$ Pa), the total inside length of the cradle (1483 mm) and the area of the Sitalls (11.6 cm^2). Assuming the 171 mm of non-Sitall FR4 end pieces act like the 1324 mm of Sitall, one gets a calculated slope of $2.24 \times 10^{-2} \mu\text{m}/\text{N}$. The slope of the measured compression in Fig. 10 is even less, only $(1.35 \pm 0.12) \times 10^{-2} \mu\text{m}/\text{N}$. This test should only be taken to indicate that our operating force of 1470 N on each Sitall column is reasonable to properly compress the Sitalls in the nineteen modules.

A second study gave us a direct measurement of the length of the detector stack. As there is no access to the Sitall faces when the modules are compressed, four brass annuli were installed on the 40 mm long Sitalls of the dense stack base plates (visible on Fig. 3). Since these Sitalls extend ~ 30 mm beyond the FR4 gas box, there was room

1 for the 10 mm thick annuli. They were positioned
2.000 ± 0.005 mm from the ends of the Sitalls using
3 precision spacers.

4 These surfaces were then accessible on the
5 upstream and downstream dense stack module,
6 allowing a direct measurement of most of the
7 length of the detector stack, including the target
8 module and all sixteen of the drift chamber
9 modules.

10 The distance between these upstream and down-
11 stream brass surfaces was measured using a dial
12 gauge mounted in a long aluminum tube holder.
13 This one meter long “aluminum dial gauge” was
14 obviously subject to temperature changes and
15 needed calibrating. This was done by repeatedly
16 measuring the length of a calibrated custom gauge
17 block. This gauge block was 1080.030 ± 0.005 mm
18 long and made of Invar, which has a low thermal
19 coefficient of $1.5 \times 10^{-6}(\text{dL}/\text{L})/^{\circ}\text{C}$.

20 Measurements were made at 1470 N force, then
21 the two measured ~2 mm brass-Sitall distances
22 were added. This gives the total length of the
23 central 17 modules (end PCs not included). The
24 value was 1083.785 ± 0.025 mm. The calculated
25 lengths of these columns, using the measured
26 thicknesses of the Sitalls from our data base, is
27 1083.786 ± 0.002 mm. This value should be re-
28 duced by the calculated compression of the Sitall
29 column at 1 470 N, which is 24 μm. The final value
30 is 1083.762 ± 0.005 mm. The difference between
31 this and the measured value is 23 μm, within the
32 ±25 μm uncertainty.

33 This excellent agreement confirms that the
34 columns of Sitall are properly compressed and
35 we know the length of the detector assembly with a
36 precision considerably better than 50 μm. With the
37 “aluminum dial gauge” in place, the cylinder
38 forces were increased from 1470 to 2940 N and
39 the reduction in the stack length recorded. The
40 measurement of this change is more accurate; the
41 value was 27 ± 5 μm. This is in a good agreement
42 with calculated value of 24 μm.

43 Knowledge of the detector stack length within
44 50 μm means that relative position of each 4 mm
45 Sitall in the stack is known with a precision of a
46 few microns, an accuracy much higher than is
47 required.

9. Gas system

49 Helium/nitrogen (~ 97:03) flows through the
50 cradle and between the modules, and the first and
51 last cathode foils in each module act as the module
52 gas windows. Two gas systems are required for the
53 TWIST modules, one for the DME gas of the 16
54 DC modules, the second for the CF₄/isobutane gas
55 for the target and the two PC modules (T+PC).
56 These gas systems are required to provide stable
57 gas flows to each of the 56 individual detectors
58 while maintaining a very low differential pressure
59 between the modules and the helium/nitrogen gas
60 of the cradle.

9.1. Description

61 Flow control for the DC system is provided by a
62 pressure regulated input manifold feeding DME
63 through 44 precision needle valves to the 44
64 individual detector layers. Each of the 44 input
65 flows is continuously monitored by inexpensive
66 mass flowmeters. The pressure between the com-
67 mon DC output manifold and the cradle gas is
68 measured with a precision differential pressure
69 transducer. This transducer signal is used to adjust
70 the output flow to the DME system output pump,
71 thus realizing differential pressure control. To
72 ensure all sixteen DC modules have a common
73 differential pressure with respect to the cradle, the
74 short neoprene bellows (~0.8 cm² × 7 cm) connect-
75 ing the outputs to the manifold, and the output
76 manifold itself (~10 cm² × 140 cm), have very low
77 flow impedance. Solenoid valves preceding the
78 DME input manifold and following the outlet
79 manifold allow the 16 DME modules to be
80 isolated, to provide protection against accidental
81 over or under pressure. These valves are pro-
82 grammed to close if the differential pressure
83 exceeds ±150 mTorr from the desired setpoint
84 pressure. A pressure relief bubbler is also set to
85 vent at ~500 mTorr with respect to atmosphere,
86 providing a final “fail safe” protection.

87 The flow and pressure control features of the
88 (T+PC) gas system are identical to the DC gas
89 system described above. The only differences are
90 that the gas is CF₄/isobutane (80:20), there are
91 only 12 detector layers (4 in the target and 4 in

each of the two PC modules), and a lower quality differential pressure transducer is used. Because CF_4 is an expensive gas, 80% of the chamber output flow is filtered, mixed with the incoming fresh supply, and recycled.

The helium/nitrogen (97:03) gas is supplied from a pressure regulated source and uses a simple mechanical flowmeter with a manual needle valve. The flow rate is typically 1 l/min to the cradle. The helium/nitrogen from the cradle is exhausted through a 1" diameter copper tube to vent at an elevation 99 cm below the midplane of the modules. The low impedance output tube is necessary to reduce cross coupling of pressure fluctuations between the (T+PC) and DC pressure control systems that can result from pressure fluctuations being transmitted through the windows of the modules of one system, through the cradle gas and into the windows of the modules of the other system. Venting the cradle gas to atmosphere 99 cm below the midplane creates a static overpressure of ~ 80 mTorr with respect to atmosphere at the modules' midplane. A pressure relief bubbler, identical to those used in the (T+PC) and DC gas systems, provides protection against accidental over pressuring of the cradle.

9.2. Pressure control

A significant challenge for the gas system design was to maintain the external cathode foils as flat as possible and with a positional stability of $\pm 50 \mu\text{m}$ or less. There are three sources of differential pressure that can deflect the module windows:

- (1) Electrostatic pressure due to the anode-to-cathode electrostatic attraction.
- (2) Gravitational pressure due to the vertical orientation of the cathodes and the difference in density between gases on either side of the first and last cathodes of each module.
- (3) Gas pressure applied by the gas supply systems.

To minimize the impact of all three effects, it was necessary to make the foil tension as high as was practical. Preliminary tension tests of stretched 339 mm diameter, $6.3 \mu\text{m}$ (nominal) thick

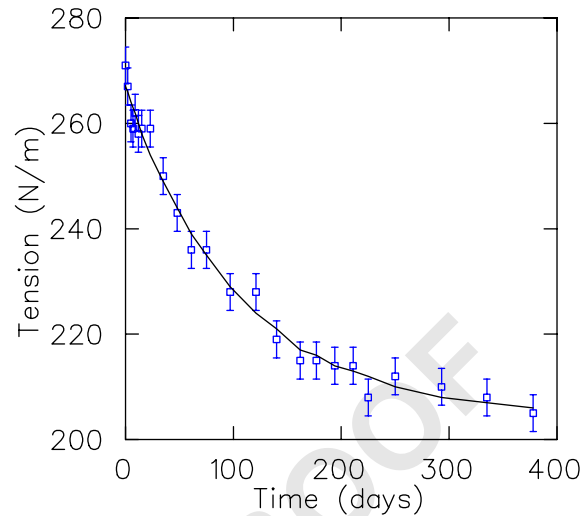


Fig. 11. Exponential relaxation of tension after $6 \mu\text{m}$ aluminized Mylar cathode foil is stretched and glued. Foil tension relaxes to 206 N/m (77% of its original value) with an exponential time constant of 102 days.

foils (doubly aluminized) revealed that after being stretched and glued to the cathode frame, the foil tension relaxes exponentially with a time constant of ~ 100 days, to an asymptotic value $\sim 75\%$ of the initial tension. Fig. 11 shows the relaxation of a test foil.

The first 59 production cathode foils were stretched to an initial tension of $\sim 340 \text{ N/m}$. Due to concerns of foils ripping from the high tension, the final 107 cathode foils were stretched to a lower initial tension of $\sim 255 \text{ N/m}$. After gluing to the cathode frame, the tension in each foil was measured and the expected final relaxed tension was calculated. From these measurements, the average expected final tension of all the foils was calculated to be $206 \pm 20 \text{ N/m}$.

A tension of 206 N/m corresponds to an average foil deflection rate of $4.7 \mu\text{m/mTorr}$, at the center of the circular foil. This implies that to keep the position of the center of the foils stable to $\pm 50 \mu\text{m}$, we would need to keep the differential pressure across the window foils constant to $\pm 11 \text{ mTorr}$.

After assembly, the pneumatic capacity of each module was measured by flowing gas into the closed module and monitoring the resulting rate of change of pressure. Pneumatic capacity (C) is

1 defined by $F = CdP/dt$, where F is the volume
 2 flow rate at STP and dP/dt the rate of change of
 3 pressure in the closed volume. From these
 4 measurements, we calculated the average tension
 5 of the window foils of each module and the
 6 average deflection rate of these foils (dz/dP). The
 7 average measured capacity of the 19 TWIST
 8 modules was 0.40 ± 0.02 cc/mTorr corresponding
 9 to an average tension in the foils of 221 ± 11 N/m,
 10 and a deflection rate of 4.5 ± 0.2 μ m/mTorr.

11 Since roughly one year (~ 3.5 tension-decay time
 12 constants) passed between the initial foil tension
 13 tests and their final assembly into modules, the
 14 results of the initial foil tension tests and the
 15 module tests are consistent.

16 The total capacity of the 16 DC modules (in the
 17 cradle) was also measured several times during
 18 various running periods of the TWIST spectrom-
 19 eter. A repeatable pattern emerged. After one
 20 day of exposure to DME the total capacity would
 21 be ~ 11 cc/mTorr. The total capacity would con-
 22 tinue to increase over the next few weeks until it
 23 stabilized at ~ 16.5 cc/mTorr, significantly higher
 24 than the expected $16 \times 0.4 = 6.4$ cc/mTorr. After
 25 exposure to air or argon for a few weeks, the total
 26 capacity would again decrease to ~ 11 cc/mTorr.
 27 The DC operating total capacity of 16.5 cc/mTorr
 28 implies an average foil deflection rate of
 29 11.6 μ m/mTorr, which requires a differential
 30 pressure stability of ± 4.3 mTorr to maintain foil
 31 position stability of ± 50 μ m.

32 The total capacity of the target and two PC
 33 modules was also measured during the various
 34 running periods. Total capacity appeared to be
 35 stable at ~ 1.45 cc/mTorr regardless of time of
 36 exposure to CF_4 /isobutane, argon/isobutane, or
 37 air. This is slightly higher than the expected total
 38 capacity of $3 \times 0.4 = 1.2$ cc/mTorr, and implies an
 39 average foil deflection rate of ~ 5.4 μ m/mTorr.

40 From these results, in particular the responses to
 41 the different gas mixtures, we suspect that the
 42 DME is being absorbed by the Mylar foils of the
 43 DC modules, causing the foil tension to relax.
 44 Some of this relaxation appears to be permanent.
 45 Bagaturia et al. [12] have also noticed foil
 46 relaxation associated with DME. In their case,
 47 the foils were Kapton GEM detectors.

The three sources of differential pressure listed
 earlier are:

(1) Electrostatic pressure: a calculation of the
 anode-cathode electrostatic attraction indi-
 cates it is equivalent to a differential pressure
 of approximately 3 mTorr for the DCs and
 7 mTorr for the PCs. These attractions are
 easily corrected by adjusting the applied
 differential gas pressure of the DC and PC
 gas systems.

(2) Gravitational pressure: The difference in den-
 sity between the detector gas and helium/
 nitrogen mix in the cradle creates a differential
 pressure across the first and last cathode foils
 of each detector module. For the DCs, this
 gravitational pressure changes by 42 mTorr
 from the top of the cathode foil to the bottom
 ($\Delta y = 340$ mm). For the PC it changes
 79 mTorr. The best compensation, is to adjust
 the applied differential gas pressure such that
 the total differential pressure (including elec-
 trostatic) is zero at the midpoint of the foil.
 The maximum pressures are then ± 21 and
 ± 40 mTorr, respectively. The gravity-induced
 pressure gradient will cause each modules'
 outermost cathode foils to bulge in towards the
 anode wires in the top half of the cathode foil,
 and bulge out away from the anodes in the
 bottom half. Since the foils are glued to
 circular FR4 rings beginning at $r = 170$ mm,
 calculating the deflections from these forces is
 quite difficult. We have estimated these deflec-
 tions, using simplifying assumptions and the
 average foil tensions calculated from the
 measured DC and PC capacities. The esti-
 mated deflections are approximately ± 30 μ m
 for the DCs, and ± 27 μ m for the PCs.

(3) Gas pressure: a high precision pressure trans-
 ducer is used to measure the differential
 pressure between the DC modules and the
 cradle gas. At our typical operating differential
 pressure the manufacturer's specifications im-
 ply a temperature drift of 0.023 mTorr/ $^{\circ}$ C.
 This is sufficient for our requirements, where
 typical extremes of temperature are less than
 ± 6 $^{\circ}$ C. The foil stability requirements for the
 target and PCs are considerably less strenuous

and consequently a less precise (and less expensive) pressure transducer is used on the (T+PC) system. The manufacturer's specifications indicate a temperature drift of $1.08 \text{ mTorr}/^\circ\text{C}$ for this gauge at our typical operating differential pressure.

For each gas system, the output signal from the pressure transducer is connected to a PID controller that in turn controls the output mass flow controller (MFC) preceding the exhaust pump, thereby controlling the differential pressure between the modules and the cradle volume. As shown in Fig. 12, the control stability obtained is about $\pm 0.5 \text{ mTorr}$. Thus, the combined transducer temperature drift and control instability contribute an error less than $\pm 1.0 \text{ mTorr}$ for the DC system, corresponding to only $\pm 12 \mu\text{m}$ foil stability. Unfortunately, these are not the only sources of differential pressure instability.

Space constraints and high magnetic fields around the cradle required that the pressure transducers be located several meters from the measurement points. "Blind" $0.25''$ OD copper tubes that traverse rising, horizontal and falling sections, connect the transducers to their measurement points. These three pressure sensing tubes are initially flushed out with the appropriate gas mixtures (DME, CF_4 /isobutane, or helium/nitrogen) and then left closed at the pressure transducer end. Accurate knowledge of the differential pressure at the center of the chambers depends on accurate knowledge of the gas density in these

tubes. A 1% change in density due to atmospheric pressure or ambient temperature change causes a 1.1 mTorr change in the measured DC differential pressure. Since atmospheric pressure and the gas temperature at several locations in the pressure sensing tubes are monitored, these changes can be compensated for.

More problematic are changes in gas composition due to diffusion or small leaks into the pressure sensing tubes. During the 2002 running period a technique was developed for periodically measuring the gas density in the pressure sensing tubes. These measurements revealed changes of up to 40 mTorr in the actual differential pressure at the center of the window foils of the DC modules. Subsequent intensive leak checking revealed some small leaks in the pressure sensing tubes. These leaks were fixed and during the 2003 running period the actual DC differential pressure was stable to $\pm 7 \text{ mTorr}$ implying a foil position stability of $\pm 80 \mu\text{m}$.

To further improve the positional stability of the window foils, we are considering a modification, so that the three pressure sensing tubes are continuously flushed with small flows of the appropriate gas mixtures. These small flows would start at the pressure sensors, pass through the sensing lines and into the chamber gas manifolds and the cradle. Flows of $\sim 1 \text{ cc}/\text{min}$ would not cause significant flow related pressure drops in the pressure sensing tubes.

Currently we are calculating the foil deflections based on pressure, temperature and chamber capacity measurements. An independent indication of the foil deflections is desirable. We are investigating the possibility of using online TDC data from the detectors to independently monitor external cathode foil deflections.

9.3. Gas composition stability

Since helium/nitrogen cradle gas surrounds the wire chambers, diffusion of helium into the chambers is a major source of contamination. GARFIELD simulations predict that a 1% change in helium concentration in the DME (from say 1–2%) would cause roughly a 1% change in electron drift times. Preliminary tests of numerous

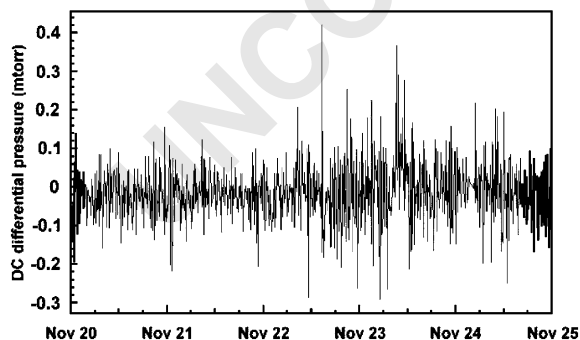


Fig. 12. Typical pressure control stability over a five day period.

pieces of 6 μm aluminized Mylar foil determined an average helium diffusion rate of $(3.6 \pm 1) \times 10^{-6} \text{ cc}/(\text{s Torr m}^2)$ or about 0.015 cc/min through each window foil. Our normal flow rate of $20 \pm 2 \text{ cc}/\text{min}$ per detector layer results in a helium concentration of 0.075% with a stability of $\pm 0.008\%$ for the (UV) modules. Since 80% of the (T+PC) gas is recycled, the helium contamination in the $\text{CF}_4/\text{isobutane}$ due to diffusion through the window foils is expected to stabilize at $(0.19 \pm 0.02)\%$.

Small leaks through pinholes in the cathode foils or holes in the module gas boxes could easily exceed diffusion through the window foils. For this reason all modules were leak checked after final assembly by filling them with helium to $\sim +500 \text{ mTorr}$ with respect to atmosphere. The inlet valve was then closed and the differential pressure to atmosphere was monitored for at least 15 minutes. Leak rates were calculated from the module's measured capacity and any resulting changes in differential pressure. Continuous measurements of gas temperature and atmospheric pressure allowed us to compensate for these effects. Only (UV), target and PC modules with measured leak rates less than 0.3 cc/min were installed in the cradle. Due to the four times higher operational total flow through dense stack (DS) modules, leak rates up to 0.6 cc/min were accepted for the DS modules. The average measured helium leak rate of the 14 (UV) modules was $0.14 \pm 0.07 \text{ cc}/\text{min}$ per module. This corresponds to an average helium concentration of 0.35% with a concentration instability of $\pm 0.04\%$ at our nominal flow rate and flow rate stability. This instability should cause a similar uncertainty of $\pm 0.04\%$ in the drift velocity, which is well within our required tolerances.

During running periods we periodically estimated the total leak rates of the DME, $\text{CF}_4/\text{isobutane}$ and cradle volumes. This was done by increasing the differential pressure in the volume to be measured by a few hundred mTorr, isolating the volume and monitoring the pressure over a period of time. These tests are sensitive to leak rates in the modules and all their connecting tubing between the isolation valves at the gas racks and the volumes under test. The measurements

were primarily used to detect changes in leak rates following reinstallation of modules. The typical measured total leak rate for the DCs (DME) was 4.5 or 0.28 cc/min module. The cradle leak rate typically measured approximately 60 cc/min. The differential pressure in the $\text{CF}_4/\text{isobutane}$ volume typically showed an increasing pressure when isolated. We suspect this effect is due to diffusion of helium or air into the detector end of the (T+PC) pressure sense line.

The $\text{CF}_4/\text{isobutane}$ (80:20) for the (T+PC) system is mixed with MFCs having a manufacturer's specified accuracy of $\pm 1\%$ of full scale. At the mixing flow rates employed, this results in a mixture of $(80 \pm 0.8)\%$ CF_4 and $(20 \pm 0.2)\%$ isobutane. Since pure DME is used for the DCs mixture accuracy is not an issue. The manufacturer's specifications for DME and isobutane supplies are 99.5% purity with typical impurities of *n*-butane and other alkanes. The CF_4 used is 99.95% pure. Oxygen contamination of all gas supplies is measured before use and typically found to be less than 20 ppm. The oxygen concentration in the exhaust gases was measured at various times during running periods. Typical oxygen concentrations were 75 ppm in the DCs, 50 ppm in the (T+PC) and 500 ppm in the cradle exhaust gas. For a 1 l/min flow through the cradle, this 500 ppm oxygen concentration implies an oxygen flow in of 0.5 cc/min, and an air leak rate of 2.5 cc/min. To compensate for this implied leak, the nitrogen content of the cradle input gas was reduced from 3% to 2.75%, so the cradle gas is actually helium/nitrogen/air (97:2.75:0.25).

10. Readout electronics

On all modules the cathode foils are grounded and positive high voltage is applied to the wires. This allows each detector layer to have its own operating voltage or to be turned off. The signals are brought through the gas box wall at high voltage and then decoupled on the preamplifier boards. Two service PCBs are mounted on each module gas box (in the readout arcs). They provide mounting and +4 V distribution for the preamplifiers.

All signal, preamplifier power, and HV cables are permanently fixed in two cable trays and sealed with a silicone rubber. The cable trays can be disconnected from the cradle and chamber stack when the detectors need to be moved out of the experimental area for service or tests (as discussed in Section 8).

We use a preamplifier developed at Fermilab for use at their Colliding Detector Facility [13]. This preamplifier is used for all the TWIST chambers and has a gain of 1 mV/fC and a dynamic range of -400 fC to $+20$ fC. Both 16 and 24 channel versions of this preamplifier are used on the detector modules.

All signals from the DCs, target and PCs go to post-amplifier/discriminators via 9.5 m long micro-coaxial cables. These custom made post-amplifier/discriminator modules have sixteen channels in a single width CAMAC unit and are housed in twelve CAMAC crates within two racks on the service platform next to the spectrometer. Each CAMAC crate contains up to 24 of these units plus a custom made controller module. This controller module interfaces with the TWIST Slow Control system and allows the adjustment of discriminator thresholds and application of test pulses. Temperature and power supply voltages are also monitored via this controller module.

The discriminator circuit produces a differential ECL logic, time over threshold output. Our operating threshold for the DC postamps is typically 150 mV. With their gain of twenty, this means a threshold equivalent to 7.5 mV at the preamp output. The VTX preamplifier has a gain of 1 mV/fC and our DC gas gain is estimated at $(1.8 \pm 0.2) \times 10^4$ (at 1950 V). This implies the effective threshold is ~ 2.5 electrons collected from a passing track. A more direct measurement indicated that detection of single electrons produced ~ 4.5 mV pulses from the preamps, so our threshold was in fact ~ 1.6 electrons. The latter is more likely, since the specified preamp gain will depend on frequency. Under these operating conditions, the noise rate was measured and found to be negligible (≤ 10 Hz/wire).

These discriminator ECL logic signals are sent to the FASTBUS TDCs (LeCroy model 1877) via 15 m long, 16-pair flat-twisted cables. The cables

are bundled and wrapped with copper laminated Mylar foil to reduce oscillations caused by RF radiation. The TDCs are multihit type and have 0.5 ns resolution. They are operated in Common Stop mode.

The FASTBUS TDCs are housed in 2 crates each containing an SIS4100NGF FASTBUS to VME interface. Each interface contains a Motorola MVME 2306 PowerPC which is responsible for transferring the TDC data to the data acquisition system [14] through an Ethernet connection. The FASTBUS crates are positioned 8 m from the service platform, to eliminate the interference from their switching power supplies.

11. Efficiency

The first efficiency tests on the drift chambers were conducted with the spectrometer magnet off, using a 120 MeV/c pion beam.

The efficiency code uses tracking information to determine which wire in a given plane is expected to display a hit. Once a track is successfully reconstructed, the track parameters are used by the efficiency algorithm to traverse through the detector stack and find the entrance and exit points of the track through each detector layer. This information is then converted into cell numbers, and the plane is searched to determine whether the TDCs corresponding to these cells (or the neighboring cells) recorded a hit. In this context, the term efficiency refers to the intrinsic efficiency of the chamber. This efficiency depends on the gas properties, cell geometry and construction (cell size, wire thickness, presence of drift wires, etc.), high voltage and threshold.

To determine an operating point for the DCs, data were obtained with the high voltage of approximately half the modules at 1900 V while the high voltage on the other half was varied from 1600 to 2000 V in steps of 50 V. Fig. 13 shows the efficiency as a function of high voltage averaged over all DC planes for which the HV was being varied. The figure insert is an expanded view of the “plateau region”, showing that the efficiency reached a value greater than 99.95%.

49

51

53

55

57

59

61

63

65

67

69

71

73

75

77

79

81

83

85

87

89

91

93

95

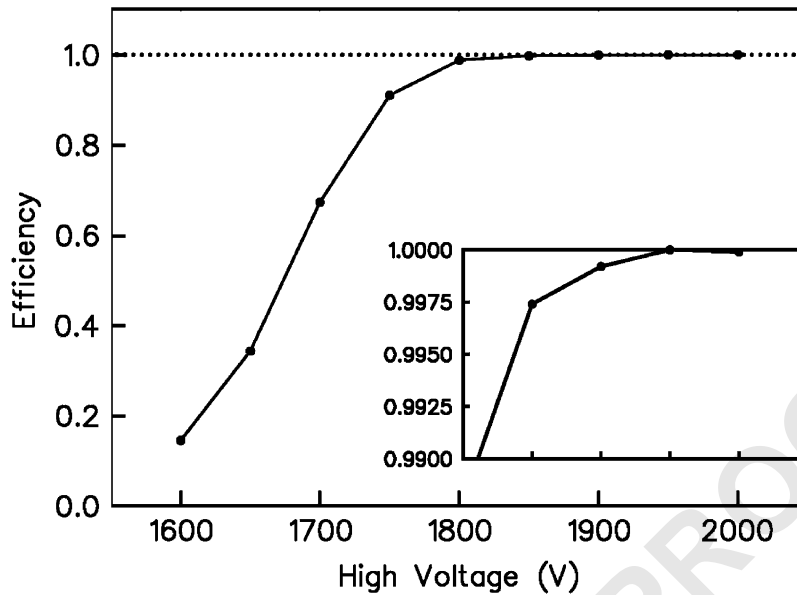


Fig. 13. DC efficiency as a function of HV.

In order to check possible plane-to-plane variations, the efficiency of each plane as a function of high voltage was calculated. Variations at 1900 V were found to be negligible, with all functioning planes showing efficiencies better than 99.8%. Differences in the shape of the efficiency as a function of high voltage in the region of interest were also found to be negligible, thereby allowing a single operating high voltage for all DC chambers. This is 1950 V. Similarly, the operating voltage of the target and PC modules was determined to be 2050 V to achieve similar, greater than 99.8% efficiencies. The wire plane high voltages are continually monitored and recorded by the slow controls system. The maximum variation is typically ± 5 V, with the DAC readout resolution being 2.44 V (12 bits = 10 kV).

Since variations in efficiency across a plane may introduce variations in energy and angular acceptance, the efficiency algorithm was also expanded to calculate a wire-by-wire efficiency. Variations in efficiency from wire-to-wire were also found negligible. The chamber efficiencies per plane are continuously monitored during data taking to ensure stability.

The algorithm used for efficiency calculations was carefully tested for possible biases. A fraction of the hits was rejected right after the unpacking of the TDCs, with the rejection factor varied by different amounts. In particular, to test the efficiency code for possible small biases, as well as sensitivities to inefficiencies of the order of 1×10^{-3} , the rejection factor was set to 0.001 and 0.002 and the difference in the calculated efficiency between the two cases was computed. This resulted in the expected efficiency difference of 0.001.

Since 120 MeV/c pions deposit more energy than muon-decay positrons, and since the Lorentz angle may in principle cause the efficiency to deteriorate when the field is on, the DC efficiency was also calculated using decay positrons at the operating high voltage of 1950 V. The results were very similar to the pion data reported above, thereby showing no deterioration in efficiency.

12. Alignment

The chamber construction techniques give a high precision in inter-plane alignments within a

1 detector layer (i.e., wire positions, foil positions,
 3 etc.), as was discussed in Section 6. The use of
 5 Sitall spacers and the cradle compression system
 7 also gives extremely high precision in the z
 9 position of the wire planes (as was discussed in
 11 Sections 2, 3, and 8).

13 However, the module assembly and mounting
 15 does not allow such a high precision in the
 17 transverse chamber positions ((x, y) or (u, v)) or
 19 rotations around the z axis. A high precision,
 21 however, is not required, since straight tracks
 23 allow for a high precision determination of both.

25 The TWIST alignment code uses 120 MeV/ c
 27 pion tracks obtained with the spectrometer magnet
 29 off to determine the transverse plane alignments
 31 and rotations around the z axis. For translational
 33 alignments, only tracks close to the center of the
 35 chamber are selected to make sure that transla-
 37 tional and rotational alignments do not mix at a
 39 significant level. Each track is fitted using a
 Kalman filter, and the means of the tracking
 residuals for each plane (except two for each
 alignment direction which are kept fixed) are used
 to adjust the transverse position of that plane. This
 process is repeated until all plane positions
 converge.

41 **Fig. 14** shows the Monte Carlo convergence of
 43 wire plane differential offsets (difference between
 45 Monte Carlo offsets and means of the tracking
 47 residuals), for the upstream 22 DC planes. The
 upper part shows the translational differential
 offsets of the tracking residuals at the end of each
 iteration for Monte Carlo data where translational
 misalignments of twice those obtained from data
 were introduced. The iteration procedure con-
 verges nicely, as is evident from the figure, and the
 precision to which the alignment code is able to
 recover these misalignments determines the accu-
 racy of this procedure to be $\sigma \sim 5 \mu\text{m}$.

For rotational alignments, the tracking residuals
 are computed in bins along the wire length, and
 the means of the tracking residuals along the wire
 length are converted into a rotation angle. This
 angle is then used to introduce a plane rotation
 correction, and the process is iterated until the
 plane rotations converge. The lower part of **Fig. 14**
 shows the rotational differential offsets at the end
 of each iteration for Monte Carlo data where

49 rotational misalignments of twice those obtained
 51 from data were introduced. The figure demon-
 53 strates convergence of the alignment process. The
 55 alignment code was also tested using Monte Carlo
 data and verified to be independent of the starting
 plane positions and independent of the alignment
 axis, defined by the fixed planes. The precision is
 $\sigma \sim 0.01^\circ$.

57 For the actual chambers, this code was used to
 59 determine the corrections for the 22 upstream DC
 61 planes and also the 22 downstream DC planes.
 63 The corrections were found to quickly converge.
 65 The derived corrections were reproducible to
 67 $\sigma \sim 5 \mu\text{m}$ for translations and $\sigma \sim 0.01^\circ$ for rotations,
 69 independent of the starting values of the misalign-
 71 ments. When the same 22 upstream DC planes
 73 were analyzed two months later, the new transla-
 75 tional corrections differed by less than $9 \mu\text{m}$ for the
 77 worst planes ($\sigma \sim 3 \mu\text{m}$). These results are quite
 79 consistent with the technique's accuracy estimated
 from Monte Carlo.

81 The required wire-plane corrections were found
 83 to vary up to $\sim 300 \mu\text{m}$ for translations and up to
 85 $\sim 0.05^\circ$ for rotations. These plane position correc-
 87 tions reflect relative plane-to-plane alignments,
 89 and their magnitude depends on the planes which
 91 were fixed to determine an alignment axis. The
 93 corrections, therefore, do not translate directly
 95 into actual plane positions. While the planes are
 expected to be positioned to an accuracy of
 $\sim 80 \mu\text{m}$ within a module, the module-to-module
 misalignments can be up to few times larger.

Since this alignment procedure requires the
 magnet to be off, calibrations runs are made at
 the beginning and end of each running period to
 ensure there are no changes. In addition, there is
 an optical alignment system on the cradle to
 monitor its position. This system uses the end of
 an optical fibre as a target. A halogen light
 illuminates the other end of the fibre and the light
 emitted from the target end is focused with lenses
 and viewed with a CCD camera element. Four
 such targets are mounted on the bottom surface of
 the cradle, two widely spaced near each endplate
 and a fifth target is near beam height and pointing
 horizontally at right angles to the beam direction
 (the $+x$ direction). These five targets are viewed
 through holes drilled in the magnet yoke. The

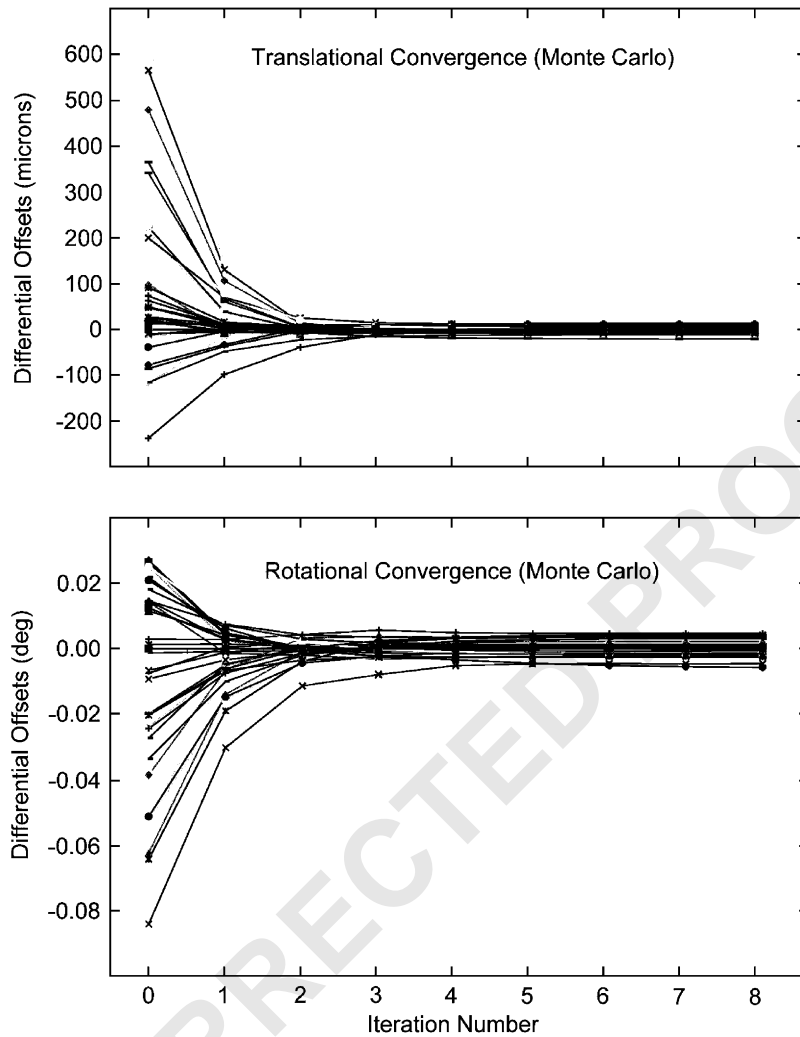


Fig. 14. Monte Carlo convergence of translational (upper) and rotational (lower) wire plane offsets, for the upstream 22 DC planes.

optical system does not touch the magnet and is firmly bolted to the concrete floor. This system indicates that the magnet and cradle system is mechanically stable to $\sim 50\ \mu\text{m}$ and not affected by the magnetic field being turned on or off.

One shortcoming of the alignment procedure using straight tracks is the inability to determine the direction of the axis of the detector relative to the direction of the axial magnetic field. However, this quantity can be determined using positron helices when the magnetic field is turned on. The

decay positron helices were used to determine this axis to better than 0.01° .

13. Resolution

As discussed in previous sections, the high precisions of the wire lane construction and the Sitall system for z positioning of the wire planes result in a negligible impact on the overall spatial resolution of the spectrometer. The transverse

plane positions (perpendicular to the z -axis), and rotations around this axis result in a significant contribution. However, once the translational and rotational corrections of each wire plane are applied, their contribution to the spatial resolution of the spectrometer are small.

There are two major contributions to the spatial resolution of the chamber; the properties of the drift cell and the mechanical precision of the detector assembly. The properties of the drift cell are mainly determined by the choice of drift gas. The high ionization density, low drift velocity and small Lorentz angle make DME a desirable choice for this experiment.

To determine the resolution of the DC planes, a subset of the upstream 22 DC planes were chosen. To define the tracks properly, but minimize multiple scattering, only 8 planes were used (four U and four V). The planes chosen were DC#7 through DC#14. These would be used to test the resolution in a ninth plane (DC#6), a V plane. DCs #6 to #8 are the last three planes in the dense stack module and the other six are the next three (UV) modules. This choice of planes means the subset spans only 188 mm (minimizing the effects of multiple scattering) and the plane not in the track fit is only 4 mm away from the first plane, so projection errors are also minimized.

As in Sections 11 and 12, we use 120 MeV/ c pion data with the magnet off. Events near normal incidence ($\theta \leq 5^\circ$) were chosen so we could map the resolution across the drift cell. For DC#7 through DC#14, events were selected that had drift distances >0.5 mm, where the resolutions were better. These tracks were fitted to a straight line and compared with the drift times in DC#6, the plane being studied. The STRs (space-time relations) started with those derived from GARFIELD, but were allowed to iterate.

Fig. 15 shows the final resolutions as a function of distance from the wire. The resolution is below $50 \mu\text{m}$ for tracks more than 1 mm from the wire, but closer than that it gets progressively worse. This deterioration in resolution closer to the wire is mainly the result of the ionization statistics.

The lower curve shown in Fig. 15 is the resolution computed from GARFIELD using a threshold of 1.6 electrons, which corresponds to

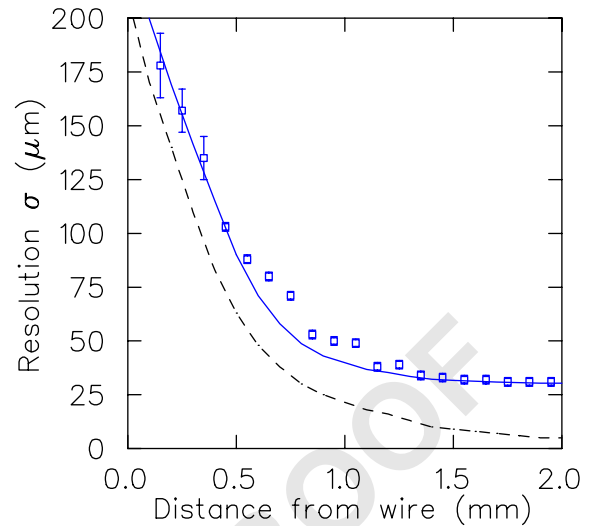


Fig. 15. Measured resolution as a function of track distance from the wire (points with error bars). The dashed curve is a GARFIELD calculation, while the solid curve also includes the quadratic addition of $30 \mu\text{m}$ spatial resolution plus 1.5 ns time resolution (see text).

our best estimate of our actual threshold (see Section 10). While it shows the resolution deteriorating closer to the wire, it predicts too good a resolution in most of the cell. This is not surprising, since this calculation does not include contributions such as: (a) residual alignment errors ($\leq 10 \mu\text{m}$) and (b) multiple scattering of the 120 MeV/ c pions over the 188 mm distance of the nine wire planes, and (c) timing jitter associated with leading edge timing and pulse height variations.

To agree with our data, we would need an added resolution contribution that was $\sim 30 \mu\text{m}$ at 1.8 mm and rises to $\sim 80 \mu\text{m}$ at 0.4 mm. For example, a multiple scattering contribution of $30 \mu\text{m}$ and a timing uncertainty of $\sim 1.5 \text{ ns}$ added in quadrature to the GARFIELD calculation produce good agreement with our measured resolutions (see upper curve in Fig. 15). Such contributions, or others, could easily account for the discrepancy.


These results were obtained with the DC chambers operating at 1900 V. Since then the operating voltages of the DCs have been raised to

1 1950 V. Since the resolution is threshold dependent, we will be collecting more test data with
 3 voltages of 1950, 2000 and 2050 V. At 2050 V, the gas gain should be $\sim 50\%$ higher.

5 Cindro et al. [15] used this technique for determining the resolution of their DME chambers.
 7 They concluded that their threshold was 10 electrons (2.0 clusters of 5 electrons each) and
 9 added a constant value of $20\mu\text{m}$ (not in quadrature) to match their observed resolution, which
 11 were only about $15\mu\text{m}$ worse than ours.

13 Fig. 16 shows the distribution of tracking residuals for DC#6. Since resolution deteriorates
 15 for tracks closer to the sense wire (Fig. 15), this distribution is only for hits having drift distances
 17 greater than 0.5mm . The distribution has $\text{FWHM} = 80\mu\text{m}$. The tails extend to $\sim 250\mu\text{m}$, and
 19 undoubtedly have contributions from; (a) multiple scattering over 188mm and 9 detector layers, and
 21 (b) hits near the 0.5mm rejection distance, where the resolution is already $\sim 90\mu\text{m}$.

23 The resolution measurements indicate that the TWIST drift chambers are giving resolutions as
 25 good as were expected.

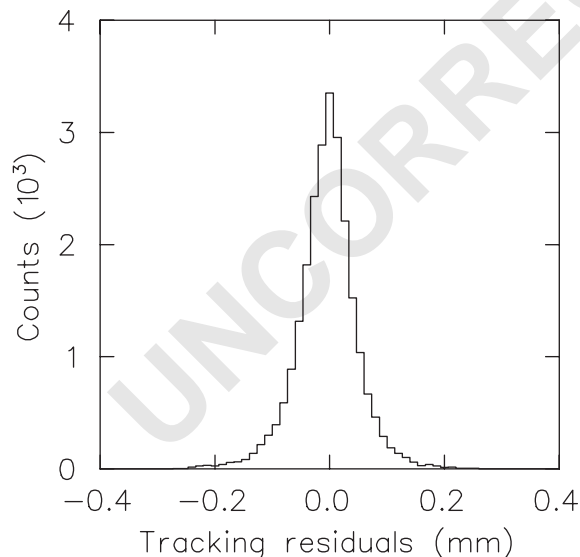

47 Fig. 16. Tracking residual distribution of DC#6, for drift distance $>0.5\text{mm}$, with FWHM of $80\mu\text{m}$.

14. Conclusions

51 The TWIST spectrometer was commissioned two years ago. There have been many calibration
 53 and data collection runs. The operation and the performance of the TWIST chambers was virtually
 55 flawless. There are no hot or dead wires in the entire spectrometer, containing 5,056 sense wires
 57 from 44 DC planes, 8 PC planes and 4 target planes. Of particular importance, the DC planes
 59 operated at full efficiency ($>99.95\%$).

61 The detector system has been extremely reliable, with only one broken wire. This required the PC
 63 module to be removed and replaced with the spare PC module.

65 Incorporating a set of low thermal expansion Sital spacers in every detector layer has resulted in
 67 a system where the z positions of each wire plane are known to a few microns and cumulative
 69 tolerances over the 120cm long tracking region are less than $50\mu\text{m}$. Using glass plate substrates
 71 for the detector layers has also resulted in a cumulative tolerance across the 320mm wide
 73 active areas of less than $\pm 6\mu\text{m}$.

75 Within each wire plane the sense wires were strung with excellent precision ($\sigma = 3.3\mu\text{m}$ in the x
 77 direction), with very few wires out of position more than $15\mu\text{m}$.

79 The mechanical system of the cradle was well designed to utilize the high quality of the module
 81 construction and to make installation and removal of modules (or even the whole cradle) as straight-
 83 forward as possible.

Acknowledgements

85 We thank the full TWIST collaboration. The design and construction of the TWIST detectors
 87 and the cradle support system could not have been accomplished without their suggestions, advice
 89 and support. D.R. Gill and N.L. Rodning, as the first two spokespersons of the TWIST collabora-
 91 tion, deserve special mention. We thank H.C. Walter and J.A. Macdonald for their contribu-
 93 tions, G. Stanford for his invaluable engineering advice and A. Prorok for his excellent design office
 95 skills. We thank C.A. Ballard, M.J. Barnes, S.

1 Chan, B. Evans, M. Goyette, D. Maas, G.M.
 2 Marshall, S. Mullin, J. Soukup, C. Stevens, P.
 3 Vincent, and L. Wampler, who contributed to the
 4 construction and operation of the TWIST cham-
 5 bers and cradle system. We also acknowledge
 6 many contributions by other members of the
 7 TRIUMF professional and technical staff. This
 8 work is supported in part by the Natural Sciences
 9 and Engineering Research Council and the Na-
 10 tional Reasearch Council of Canada, the Russian
 11 Ministry of Science, and the U.S. Department of
 12 Energy.

15 References

- 17 [1] S. Eidelman, et al., Phys. Lett. B 592 (2004) 1 (see article by
 18 W. Fetscher and H.J. Gerber, p. 410).
 19 [2] A.E. Pifer, T. Bowen, K.R. Kendall, Nucl. Instr. and
 20 Meth. 135 (1976) 39.
 21 [3] Sitall CO-115M, Northern Lights Optics 8B-186, 3110 8th
 St., E. Saskatoon, Saskatchewan S7H 0W2, Canada.
<http://www.minerals.sk.ca>.
- [4] Schott Glass Technologies, 400 York Ave, Duryea, PA 18642, USA. 23
 [5] GEANT, version 3.2114. 25
 [6] R. Veenhof, GARFIELD, a drift chamber simulation program, Version 7.10. 27
 [7] Gas Encyclopedia, L'Air Liquide Scientific Division, Elsevier, Amsterdam, 1976, p. 533. 29
 [8] R. Openshaw, R. Henderson, Nucl. Instr. and Meth. A 515 (2003) 89 (Proceedings of the International Workshop on Aging Phenomena in Gaseous Detectors, Hamburg, Germany, Oct 2001). 31
 [9] GC Electronics, EMI-RFI Shield, cat. no. 10-4807. Manufactured by: GC/Waldom Inc, 1801 Morgan St, Rockford, IL 61102-2690, USA. 33
 [10] Goodfellow Corp, 800 Lancaster Ave, Berwyn, PA 19312-1780, USA. 35
 [11] ANSYS, Inc., Canonsburg, PA. 37
 [12] Y. Bagaturia, et al., Nucl. Instr. and Meth. A 490 (2002) 223. 39
 [13] R.J. Yarema, et al., IEEE Trans. Nucl. Sci. NS-39 (1992) 742. 41
 [14] R. Poutissou, et al., 13th IEEE-NPSS Real Time Conference 2003, Montreal, May 2003. TRIUMF preprint TRI-PP-04-16. <http://www.triumf.ca/publications/pplist/pp04.html>. 43
 [15] V. Cindro, et al., Nucl. Instr. and Meth. A 309 (1991) 411.

UNCORRECTED PROOF